

Data File : S:\HPCHEM1\HPLC_L\DATA\HL070213\HL005486.D Vial: 17
Acq On : 03-Jul-2013, 02:09 Operator: QM
Sample : E2747-15 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 5 16:04 2013 Quant Results File: HL070213.RES

Instrument :
HPLC_L
ClientSampleId :
POLJAT02-SS4-062513

Manual Integrations
APPROVED

QI
7/3/2013 11:27:22 AM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 02 17:40:52 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.32	725402	179.118 ug/L

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005486.D HL070213.M

Sat Jul 06 00:05:22 2013

RPT1

Quantitation Report

Data File : S:\HPCHEM1\HPLC_L\DATA\HL070213\HL005486.D Vial: 17
Acq On : 03-Jul-2013, 02:09 Operator: QM
Sample : E2747-15 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 5 16:04 2013 Quant Results File: HL070213.RES


Instrument :
HPLC_L
ClientSampleId :
POLJAT02-SS4-062513


Manual Integrations
APPROVED

QI
7/3/2013 11:27:22 AM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 02 17:40:52 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

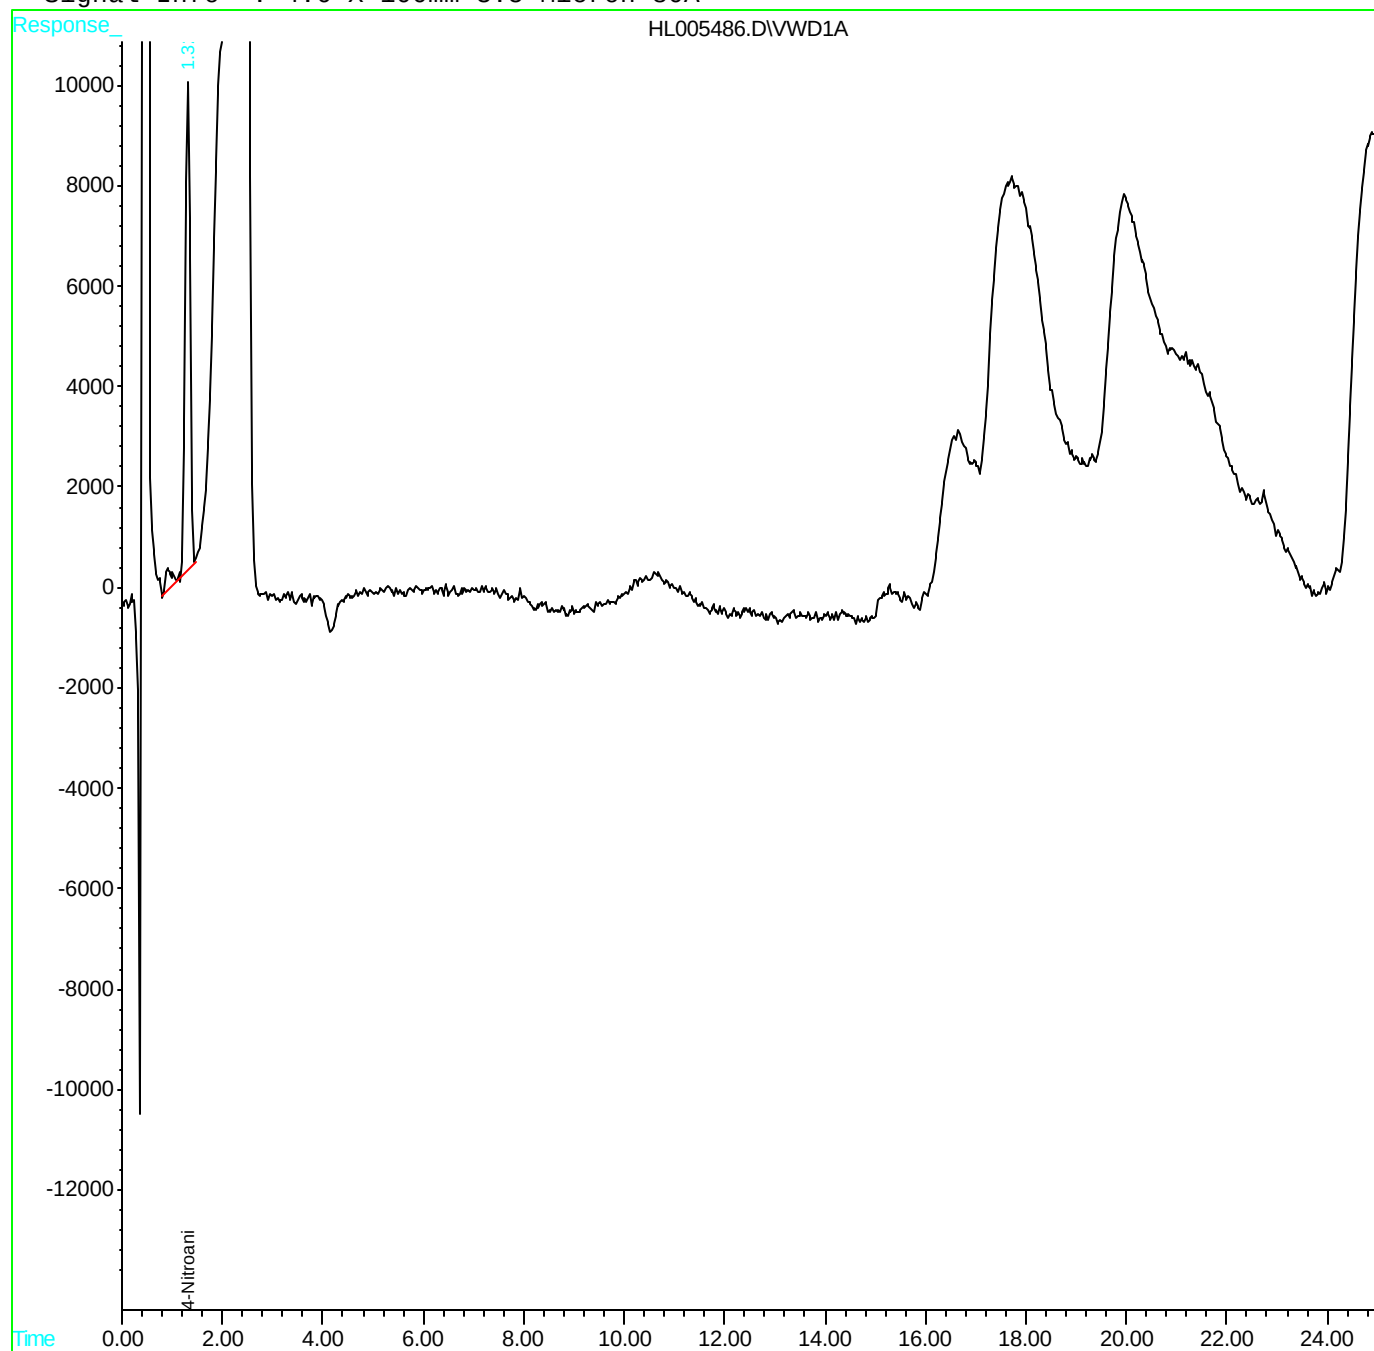

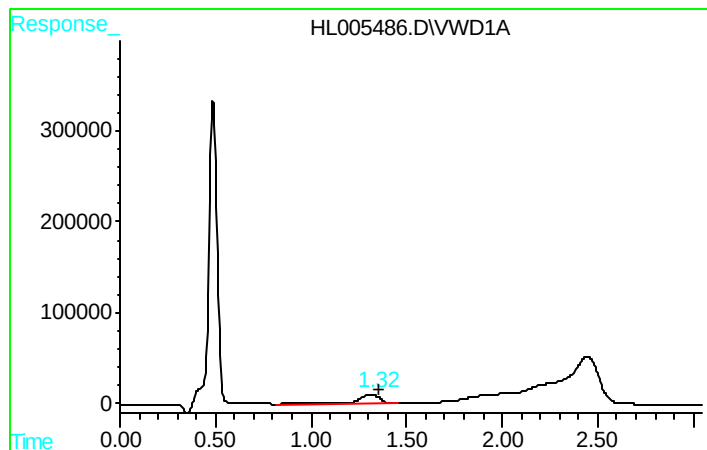

#1 4-Nitroaniline

R.T.: 1.317 min
Delta R.T.: -0.035 min
Response: 725402
Conc: 179.12 ug/L

Instrument :
HPLC_L
ClientSampleId :
POLJAT02-SS4-062513

Manual Integrations
APPROVED

QI
7/3/2013 11:27:22 AM