

Data File : S:\HPCHEM1\HPLC_L\DATA\HL070513\HL005504.D Vial: 8
Acq On : 05-Jul-2013, 17:12 Operator: QM
Sample : E2748-14 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 9 1:17 2013 Quant Results File: HL070213.RES

Instrument :
HPLC_L
ClientSampleId :
POLJAT01-SS5-062713

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 02 16:59:51 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.33	755016	186.430 ug/L
Target Compounds			
2) T HMX	0.92	314132	68.195 ug/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005504.D HL070213.M

Tue Jul 09 01:17:40 2013

RPT1


Quantitation Report


Data File : S:\HPCHEM1\HPLC_L\DATA\HL070513\HL005504.D Vial: 8
Acq On : 05-Jul-2013, 17:12 Operator: QM
Sample : E2748-14 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 9 1:17 2013 Quant Results File: HL070213.RES

Instrument :
HPLC_L
ClientSampleId :
POLJAT01-SS5-062713

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 02 16:59:51 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

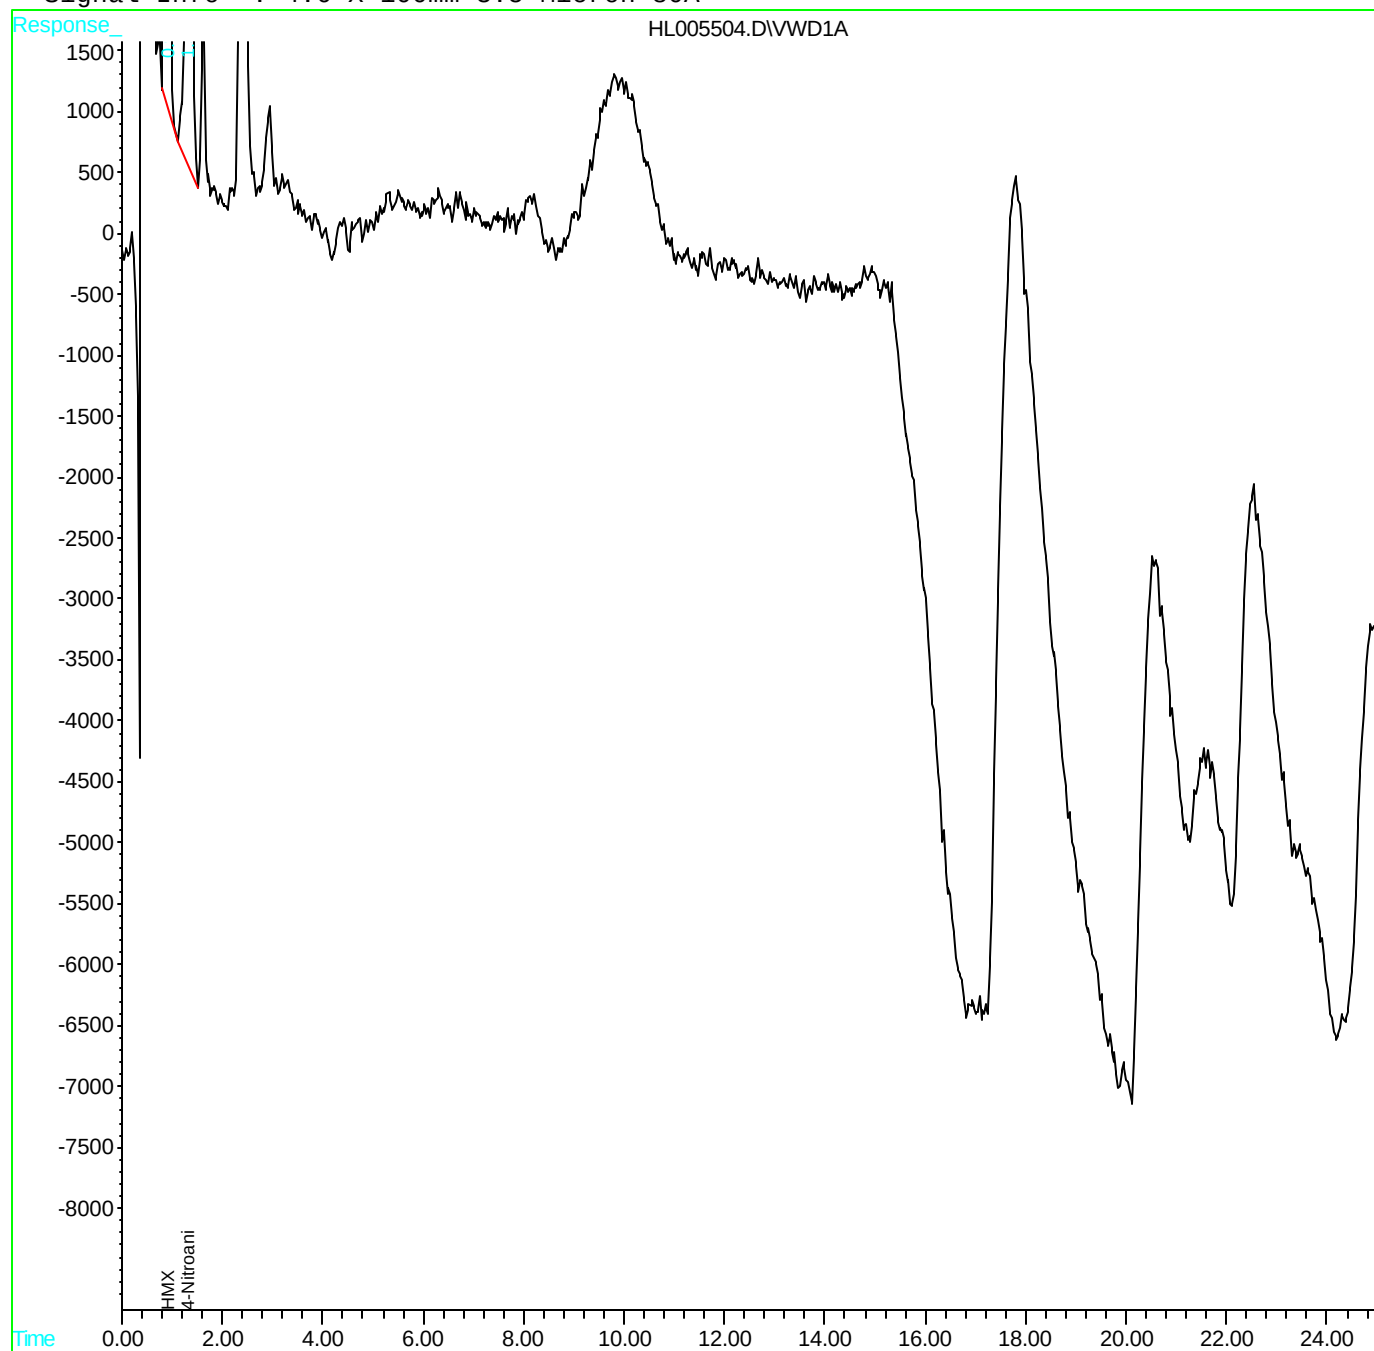


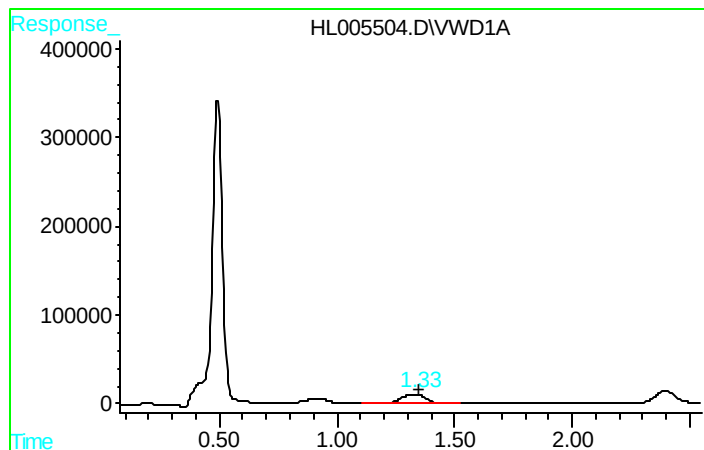

#1 4-Nitroaniline

R.T.: 1.332 min
 Delta R.T.: -0.020 min
 Response: 755016
 Conc: 186.43 ug/L

Instrument :
 HPLC_L
 ClientSampleId :
 POLJAT01-SS5-062713

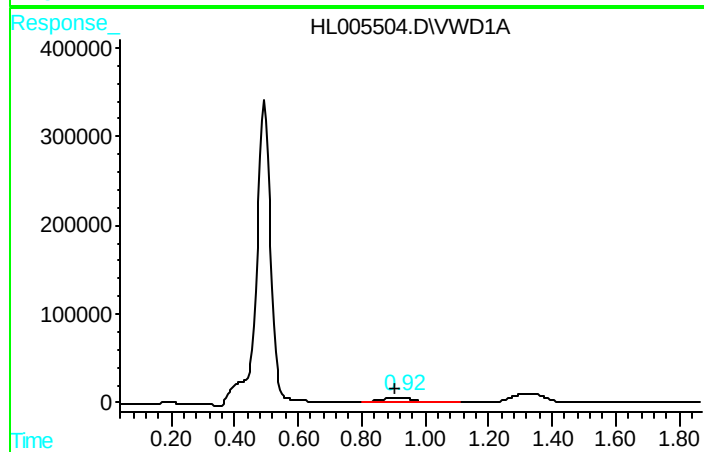

#2 HMX

R.T.: 0.921 min
 Delta R.T.: 0.018 min
 Response: 314132
 Conc: 68.20 ug/L