

Data File : S:\HPCHEM1\HPLC_L\DATA\HL070513\HL005508.D Vial: 11
Acq On : 05-Jul-2013, 19:00 Operator: QM
Sample : E2748-11 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 9 1:30 2013 Quant Results File: HL070213.RES

Instrument :
HPLC_L
ClientSampleId :
POLJAT01-SS6-062713

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 02 16:59:51 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.34	769639	190.041 ug/L
Target Compounds			
17) T PETN	19.60	649805	31.508 ug/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005508.D HL070213.M

Tue Jul 09 01:30:15 2013

RPT1


Quantitation Report


Data File : S:\HPCHEM1\HPLC_L\DATA\HL070513\HL005508.D Vial: 11
Acq On : 05-Jul-2013, 19:00 Operator: QM
Sample : E2748-11 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 9 1:30 2013 Quant Results File: HL070213.RES

Instrument :
HPLC_L
ClientSampleId :
POLJAT01-SS6-062713

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 02 16:59:51 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

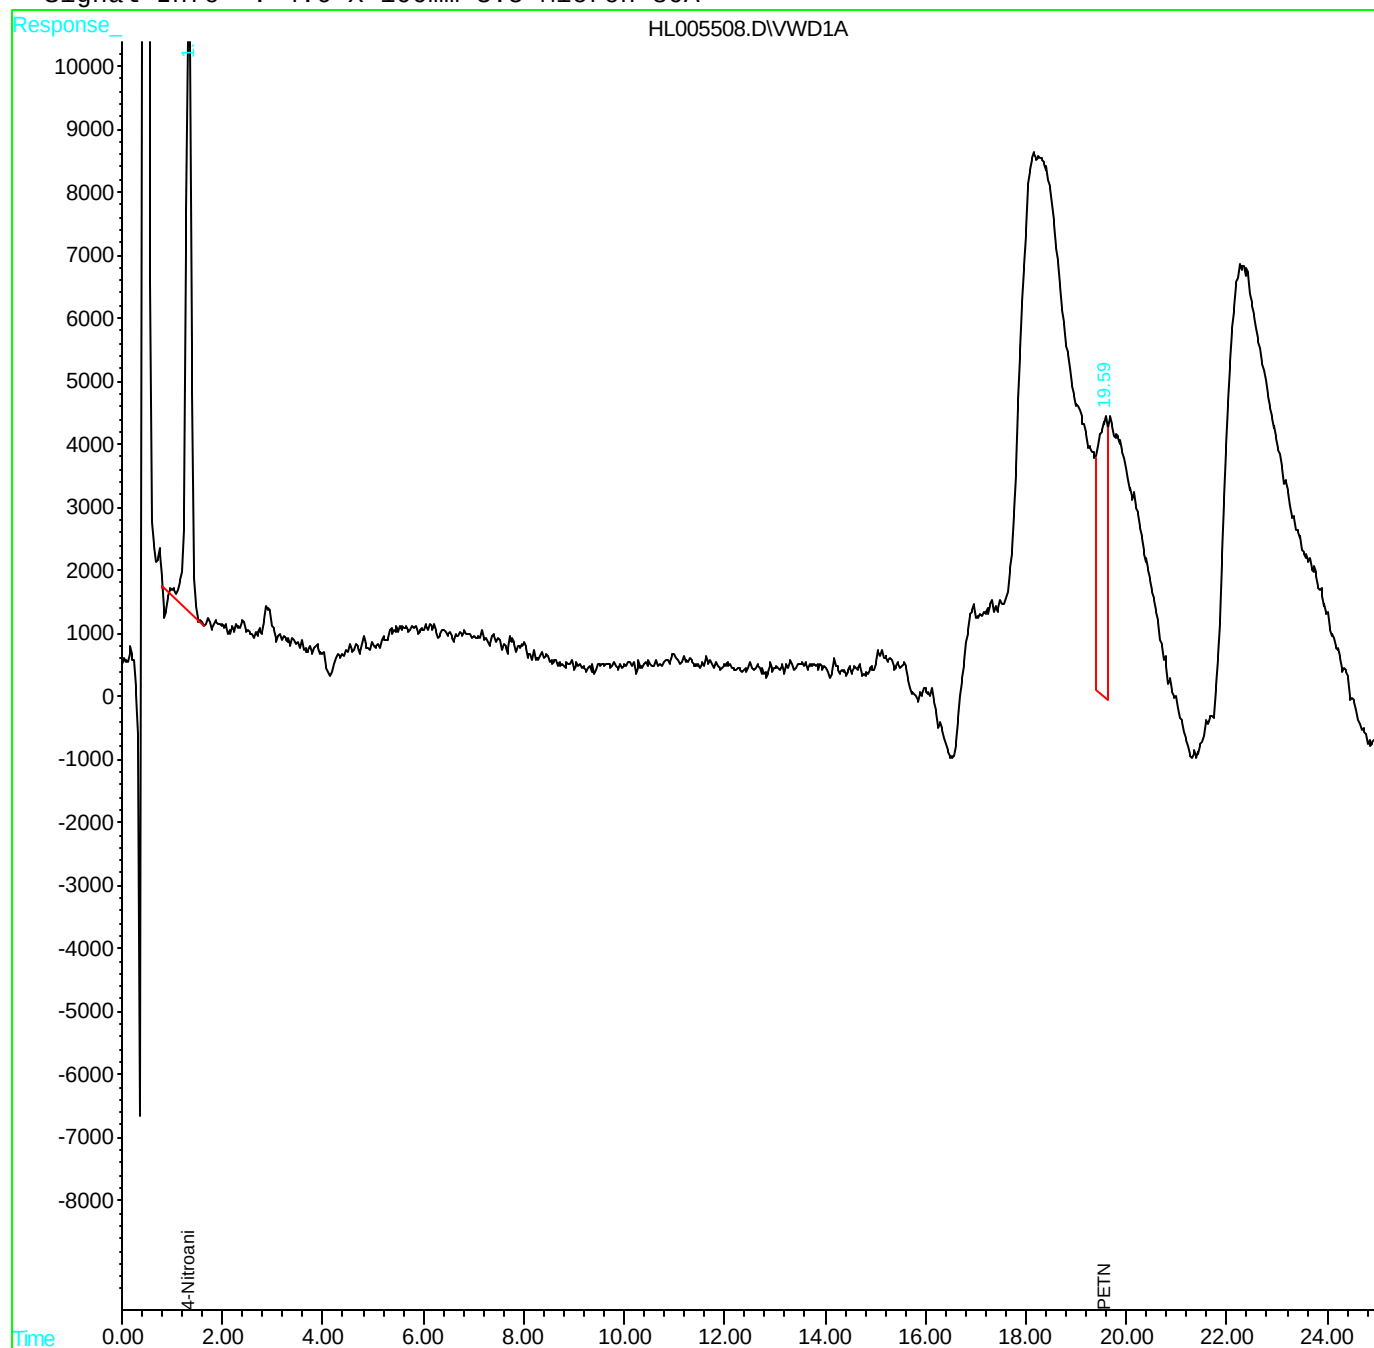


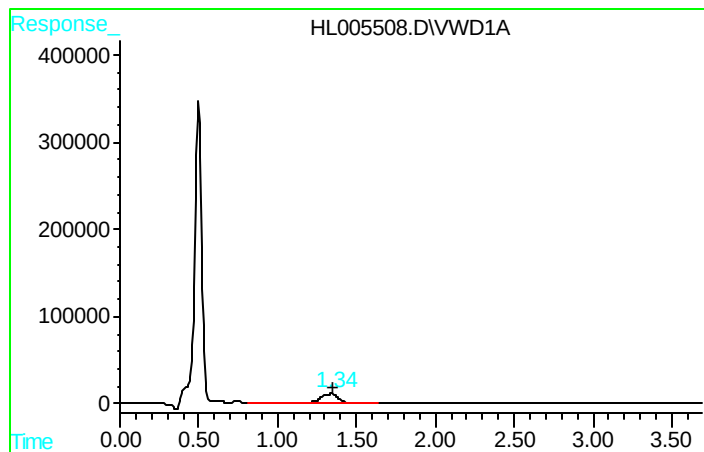

#1 4-Nitroaniline

R.T.: 1.337 min
Delta R.T.: -0.015 min
Response: 769639
Conc: 190.04 ug/L

Instrument :
HPLC_L
ClientSampleId :
POLJAT01-SS6-062713

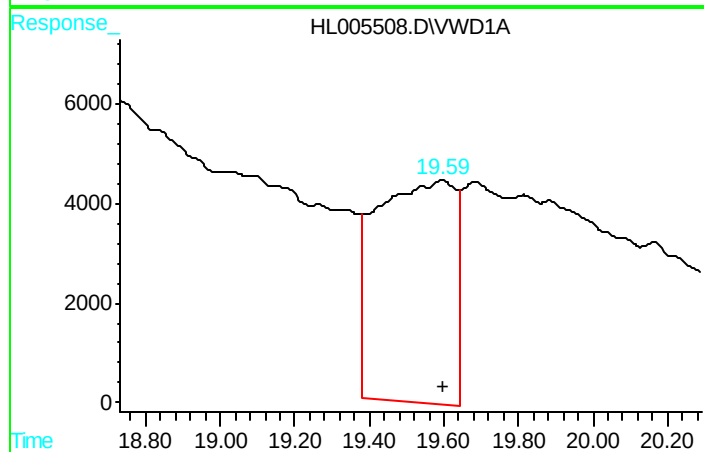

#17 PETN

R.T.: 19.596 min
Delta R.T.: -0.004 min
Response: 649805
Conc: 31.51 ug/L