

Data File : S:\HPCHEM1\HPLC_L\DATA\HL070513\HL005506.D Vial: 10
Acq On : 05-Jul-2013, 18:06 Operator: QM
Sample : E2748-12 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 9 1:21 2013 Quant Results File: HL070213.RES

Instrument :
HPLC_L
ClientSampleId :
POLJAT01-SS7-062713

Manual Integrations
APPROVED

QI
7/9/2013 4:22:44 PM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 02 16:59:51 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.35	734607	181.391 ug/L m

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005506.D HL070213.M

Thu Jul 11 23:42:33 2013

RPT1

Quantitation Report

Data File : S:\HPCHEM1\HPLC_L\DATA\HL070513\HL005506.D Vial: 10
Acq On : 05-Jul-2013, 18:06 Operator: QM
Sample : E2748-12 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 9 1:21 2013 Quant Results File: HL070213.RES


Instrument :
HPLC_L
ClientSampleId :
POLJAT01-SS7-062713


Manual Integrations
APPROVED

QI
7/9/2013 4:22:44 PM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 02 16:59:51 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

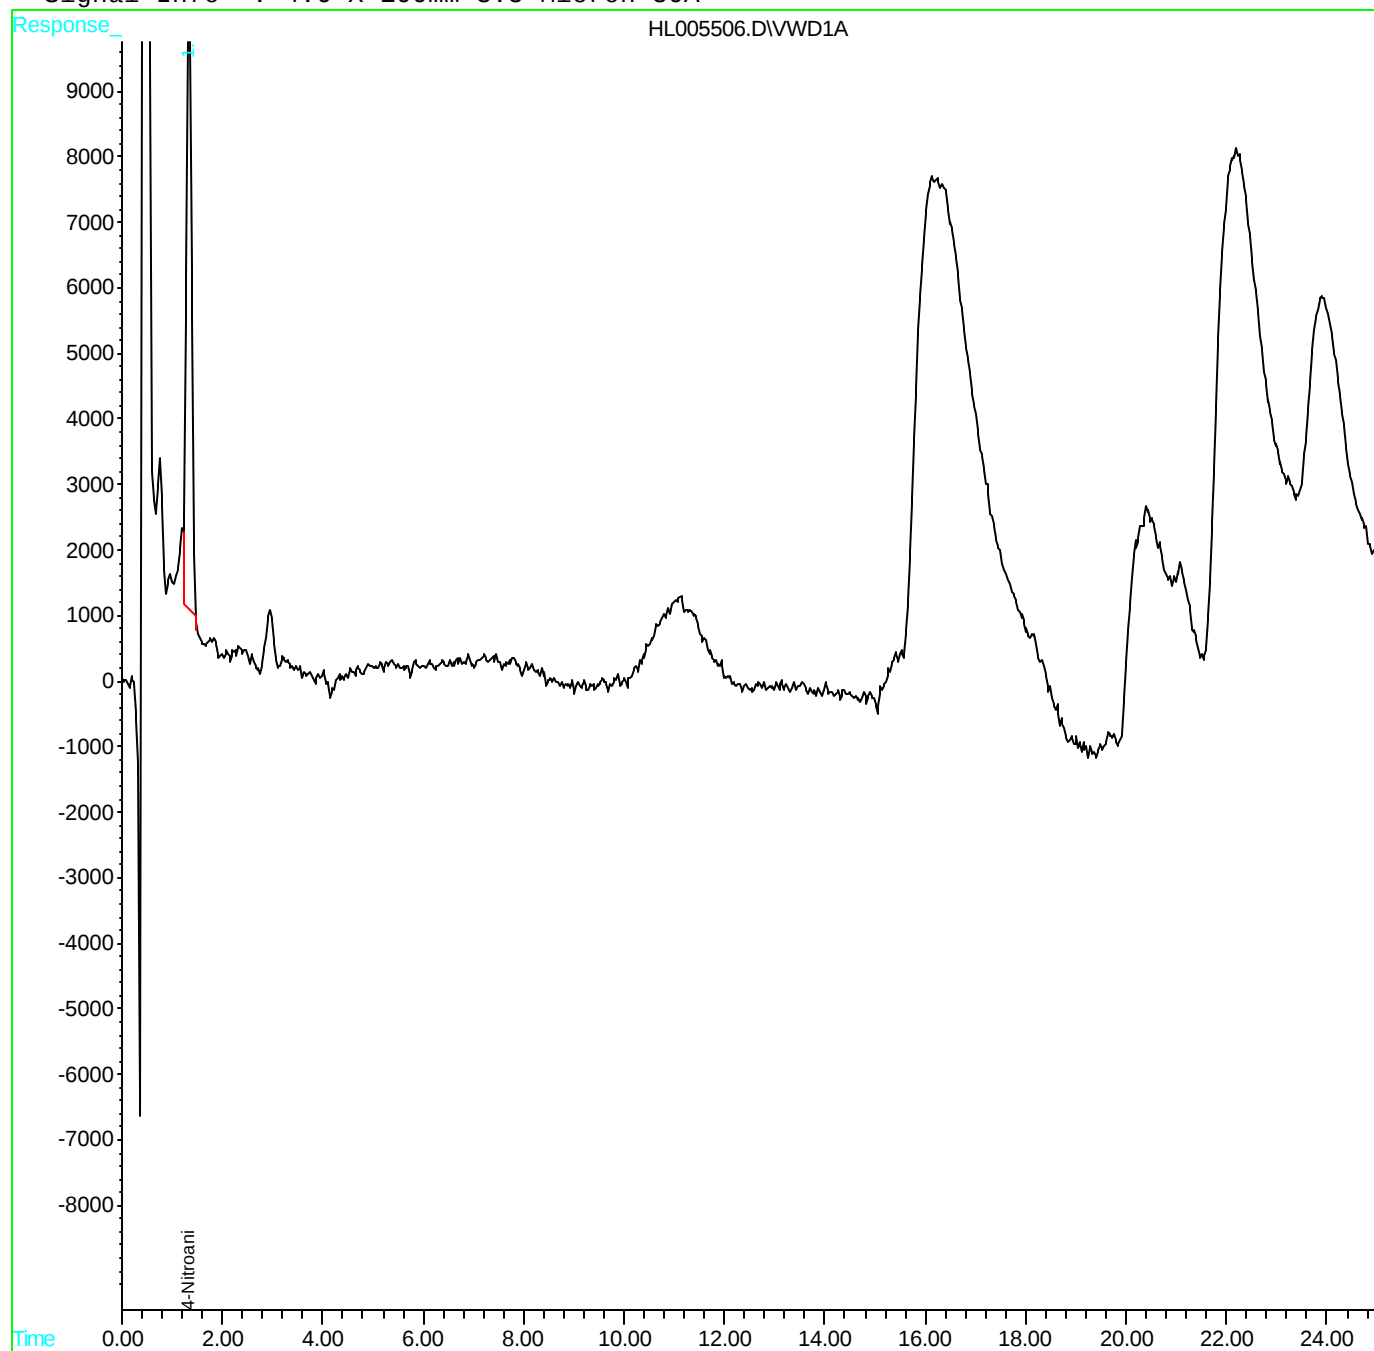

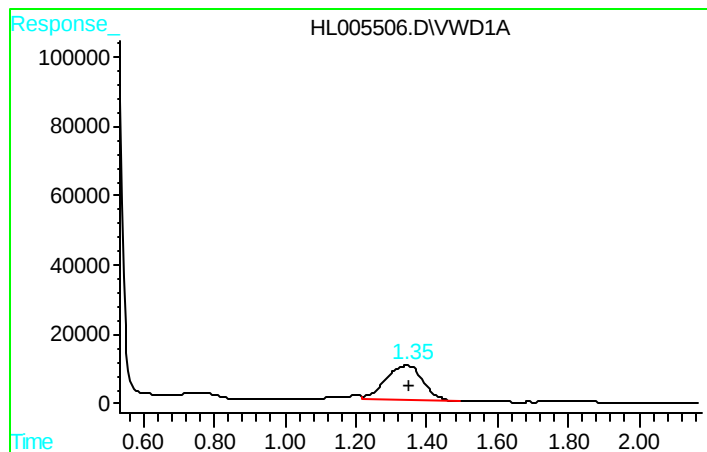

#1 4-Nitroaniline

R.T.: 1.346 min
Delta R.T.: -0.006 min
Response: 734607
Conc: 181.39 ug/L m

Instrument :
HPLC_L
ClientSampleId :
POLJAT01-SS7-062713

Manual Integrations
APPROVED

QI
7/9/2013 4:22:44 PM