

Data File : S:\HPCHEM1\HPLC_L\DATA\HL070913\HL005526.D Vial: 9
Acq On : 09-Jul-2013, 16:33 Operator: QM
Sample : E2797-04 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 9 16:59 2013 Quant Results File: HL070213.RES

Instrument :
HPLC_L
ClientSampleId :
113-MW-1

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 09 16:49:28 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	1345642	332.269 ug/L
Target Compounds			
13) T 2,6-Dinitrotoluene	8.46	343988	41.122 ug/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005526.D HL070213.M

Tue Jul 09 16:59:37 2013

RPT1


Quantitation Report


Data File : S:\HPCHEM1\HPLC_L\DATA\HL070913\HL005526.D Vial: 9
Acq On : 09-Jul-2013, 16:33 Operator: QM
Sample : E2797-04 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 9 16:59 2013 Quant Results File: HL070213.RES

Instrument :
HPLC_L
ClientSampleId :
113-MW-1

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 09 16:49:28 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

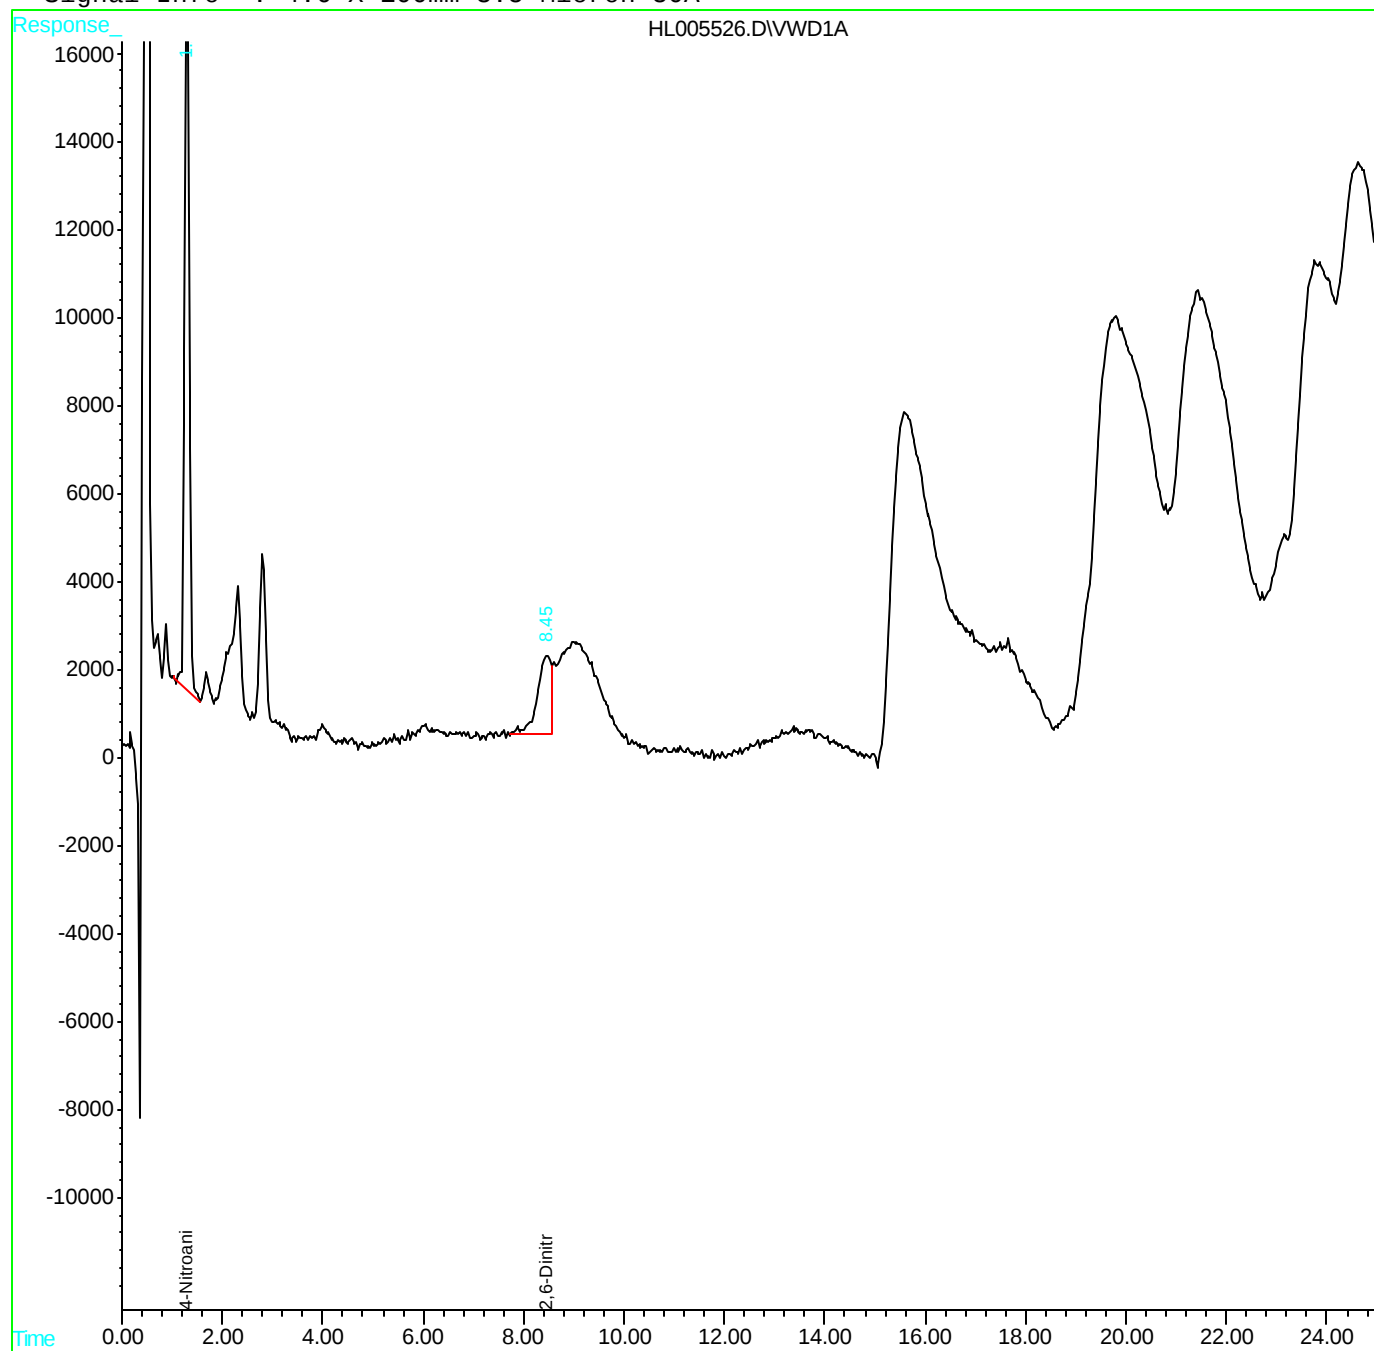


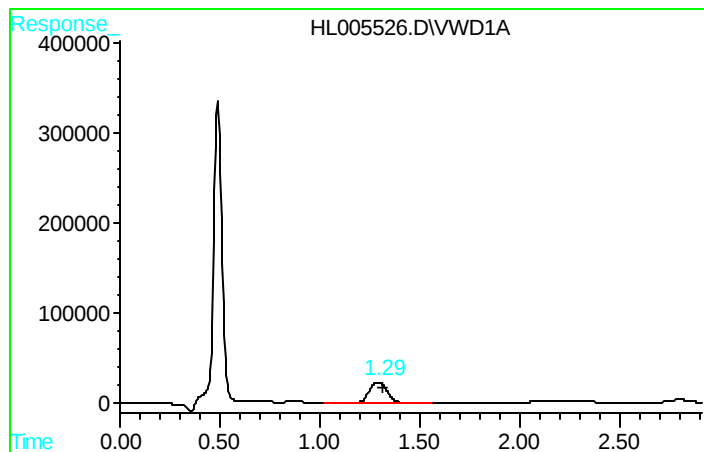

#1 4-Nitroaniline

R.T.: 1.295 min
Delta R.T.: -0.025 min
Response: 1345642
Conc: 332.27 ug/L

Instrument :
HPLC_L
ClientSampleId :
113-MW-1

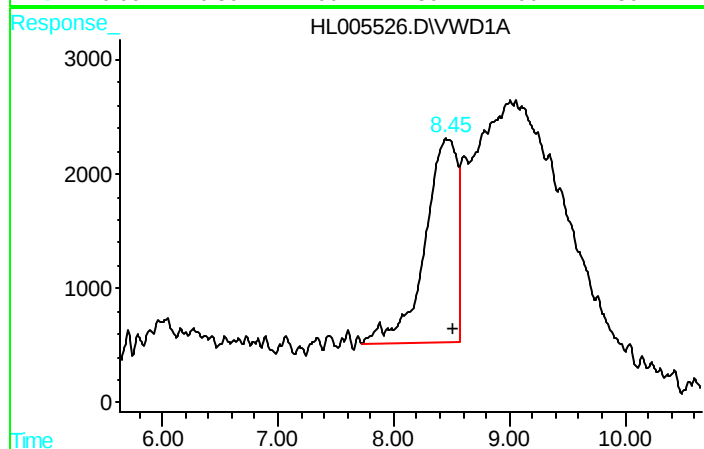

#13 2,6-Dinitrotoluene

R.T.: 8.461 min
Delta R.T.: -0.045 min
Response: 343988
Conc: 41.12 ug/L