

Data File : S:\HPCHEM1\HPLC_L\DATA\HL070913\HL005532.D Vial: 14
Acq On : 09-Jul-2013, 19:15 Operator: QM
Sample : E2748-17 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 10 7:26 2013 Quant Results File: HL070213.RES

Instrument :
HPLC_L
ClientSampleId :
POLJAT01-EB-062713

Manual Integrations
APPROVED

QI
7/10/2013 9:54:39 AM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 09 17:29:55 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.27	1221808	301.692 ug/L m

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005532.D HL070213.M

Fri Jul 12 00:35:41 2013

RPT1

Quantitation Report

Data File : S:\HPCHEM1\HPLC_L\DATA\HL070913\HL005532.D Vial: 14
Acq On : 09-Jul-2013, 19:15 Operator: QM
Sample : E2748-17 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 10 7:26 2013 Quant Results File: HL070213.RES


Instrument :
HPLC_L
ClientSampleId :
POLJAT01-EB-062713


Manual Integrations
APPROVED

QI
7/10/2013 9:54:39 AM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL070213.M
Title :
Last Update : Tue Jul 09 17:29:55 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

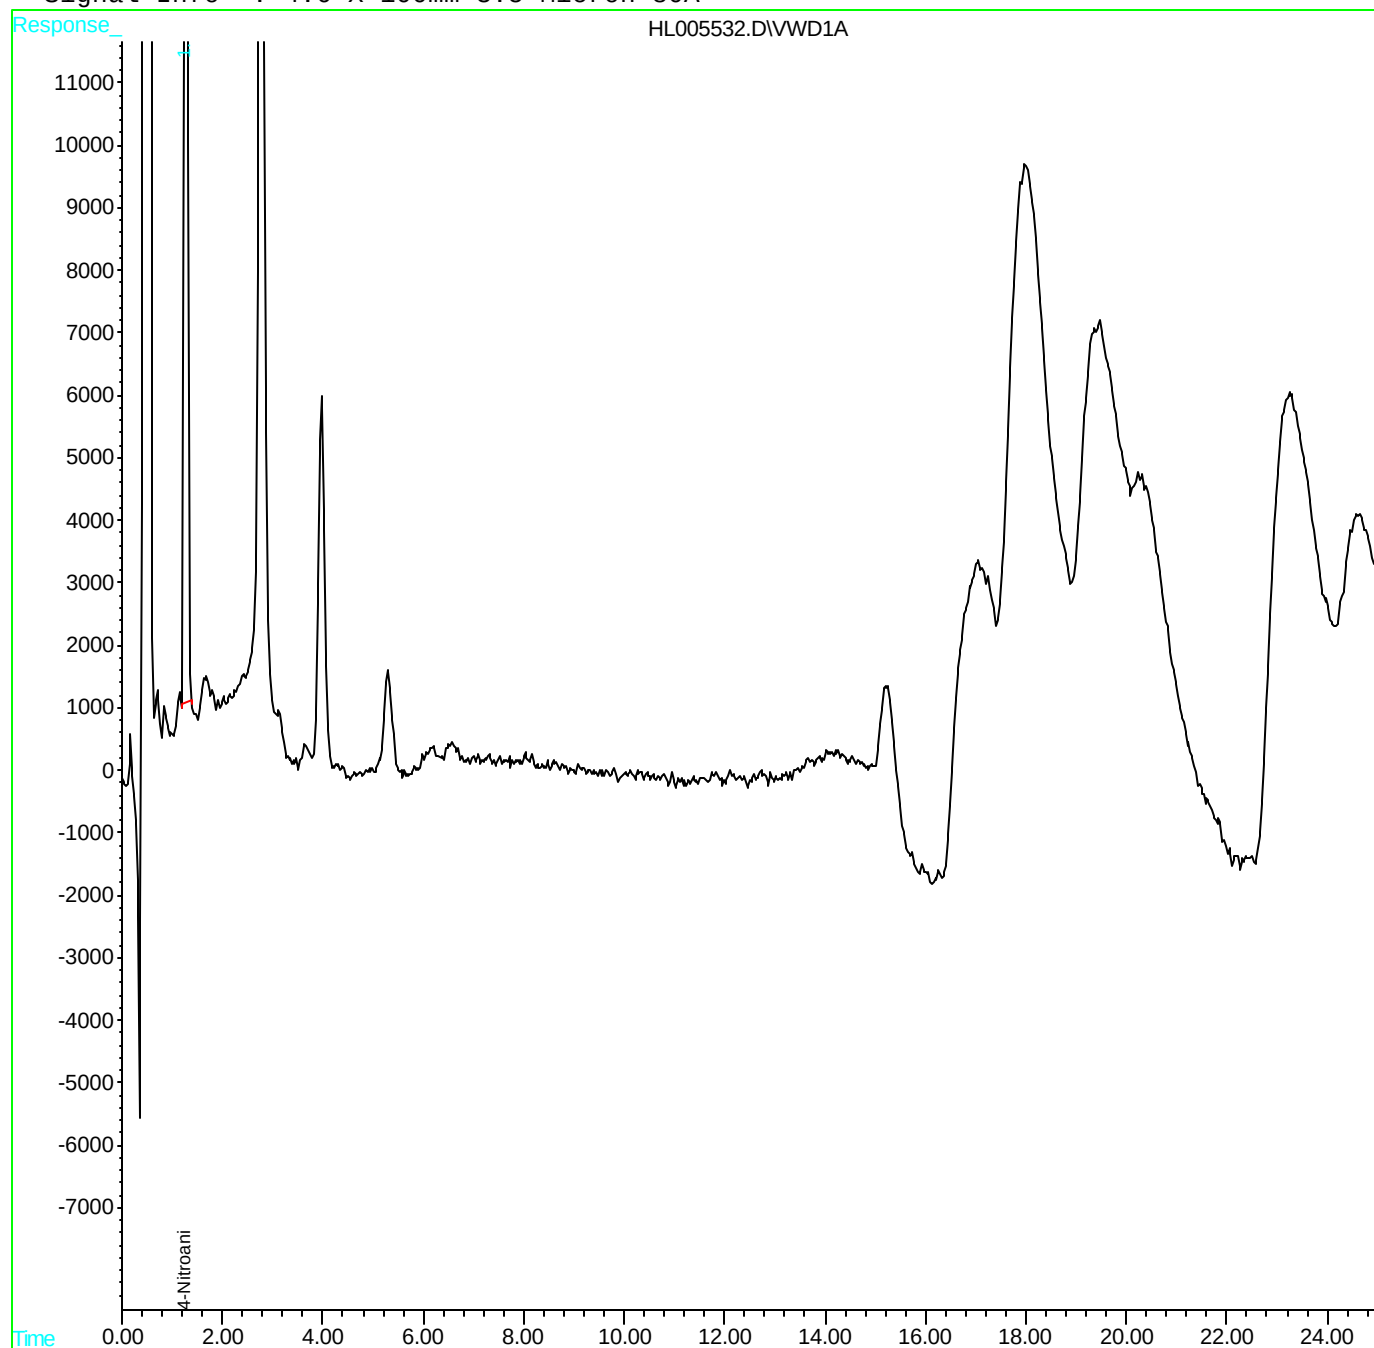

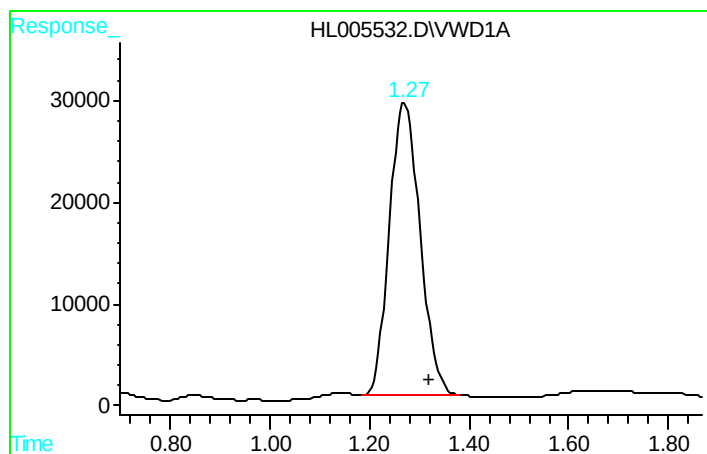

#1 4-Nitroaniline

R.T.: 1.268 min
Delta R.T.: -0.051 min
Response: 1221808
Conc: 301.69 ug/L m

Instrument :
HPLC_L
ClientSampleId :
POLJAT01-EB-062713

Manual Integrations
APPROVED

QI
7/10/2013 9:54:39 AM