

Data File : S:\HPCHEM1\HPLC\_L\DATA\HL071113\HL005549.D Vial: 16  
Acq On : 12-Jul-2013, 00:32 Operator: QM  
Sample : E2837-05 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: Jul 11 21:58 2013 Quant Results File: HL071113.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
BG500SS03A

Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL071113.M  
Title :  
Last Update : Thu Jul 11 21:31:35 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T. | Response | Conc Units   |
|-----------------------------|------|----------|--------------|
| -----                       |      |          |              |
| System Monitoring Compounds |      |          |              |
| 1) S 4-Nitroaniline         | 1.32 | 792081   | 198.860 ug/L |
| Target Compounds            |      |          |              |
| 2) T HMX                    | 0.86 | 262108   | 63.897 ug/L  |

-----  
Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005549.D HL071113.M

Thu Jul 11 21:58:50 2013

RPT1


# Quantitation Report


Data File : S:\HPCHEM1\HPLC\_L\DATA\HL071113\HL005549.D Vial: 16  
Acq On : 12-Jul-2013, 00:32 Operator: QM  
Sample : E2837-05 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: Jul 11 21:58 2013 Quant Results File: HL071113.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
BG500SS03A

Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL071113.M  
Title :  
Last Update : Thu Jul 11 21:31:35 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

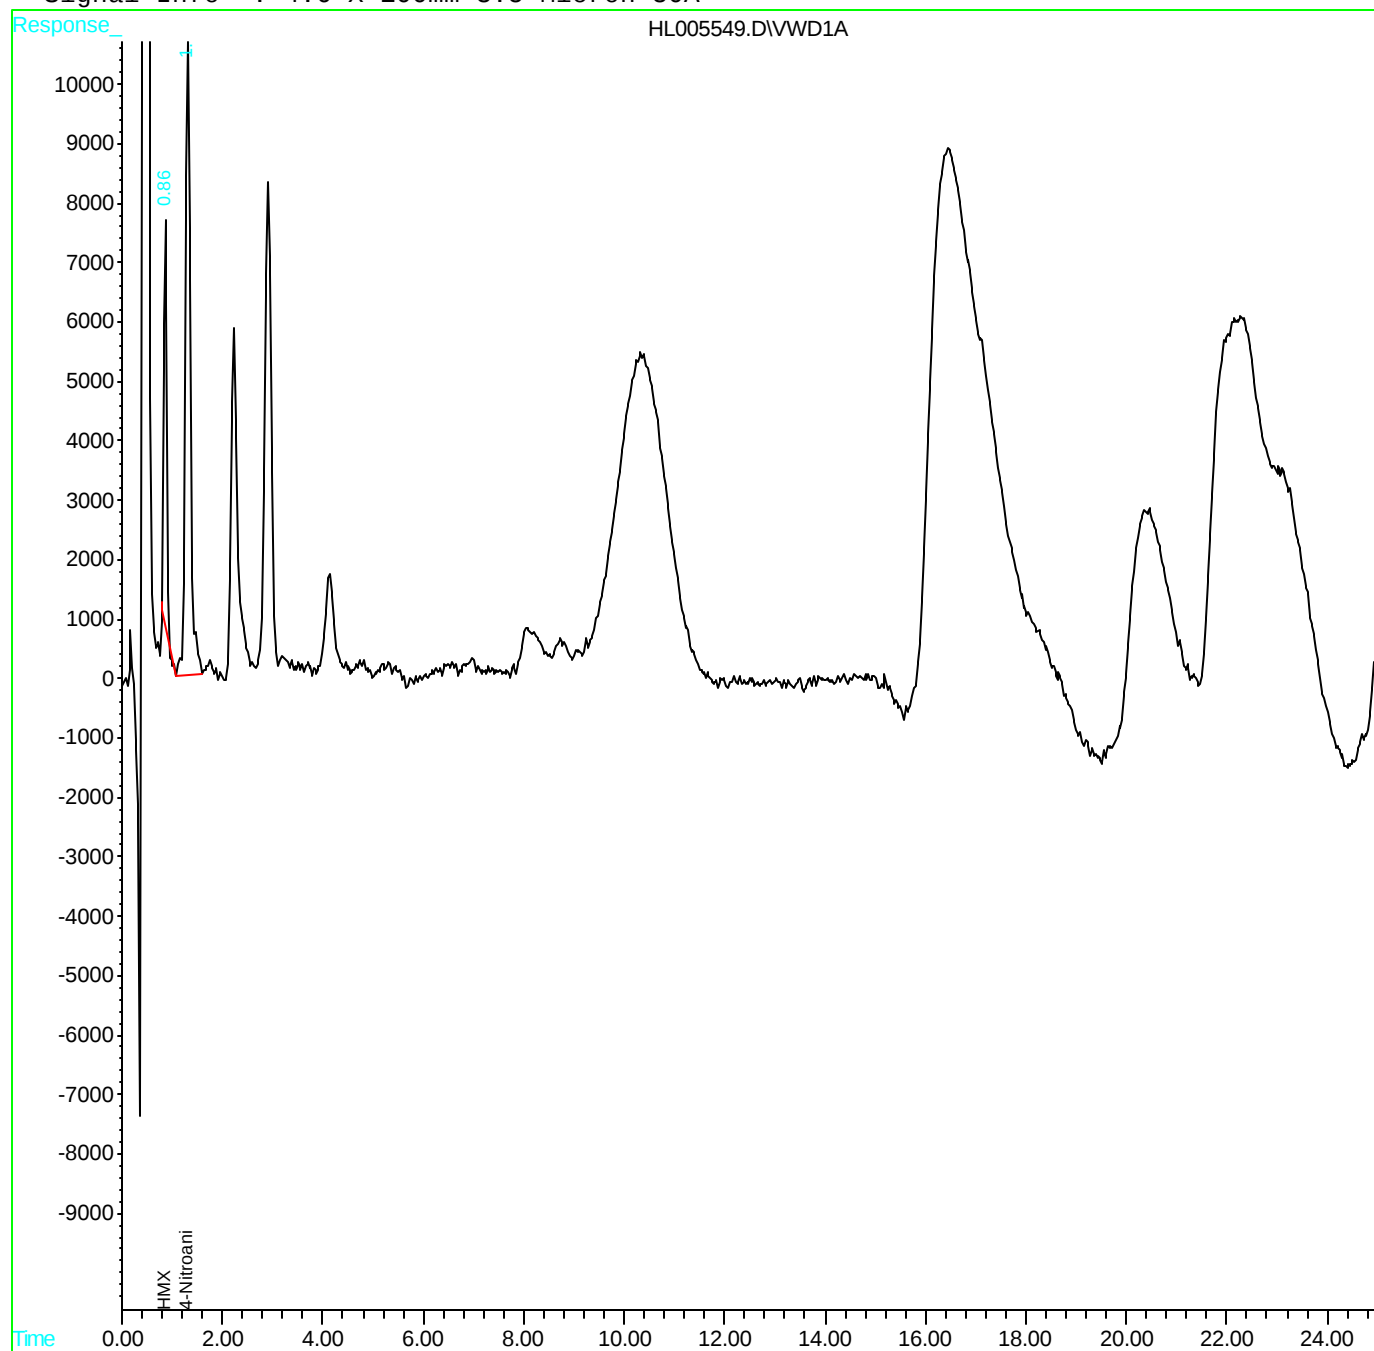


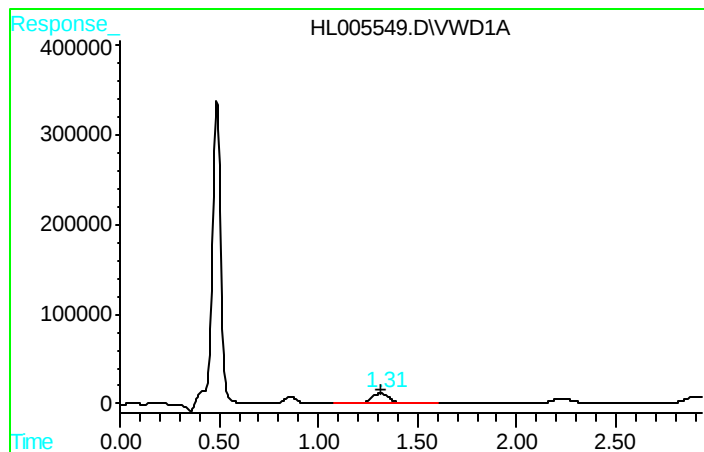

#1 4-Nitroaniline

R.T.: 1.315 min  
 Delta R.T.: -0.004 min  
 Response: 792081  
 Conc: 198.86 ug/L

Instrument :  
 HPLC\_L  
 ClientSampleId :  
 BG500SS03A

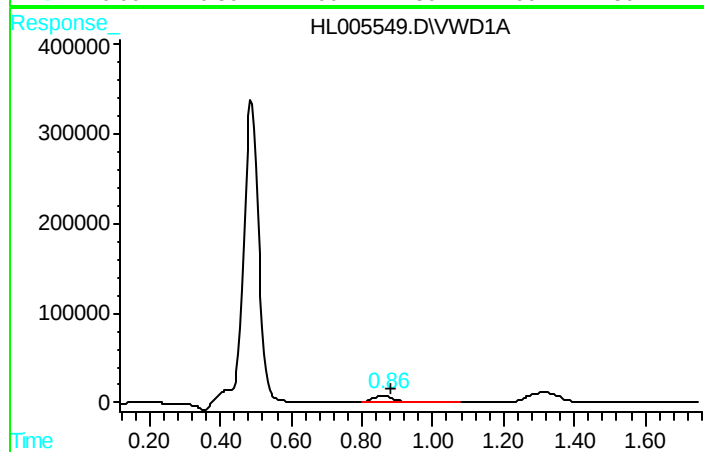

#2 HMX

R.T.: 0.862 min  
 Delta R.T.: -0.022 min  
 Response: 262108  
 Conc: 63.90 ug/L