

Data File : S:\HPCHEM1\HPLC_L\DATA\HL071113\HL005549.D Vial: 16
Acq On : 12-Jul-2013, 00:32 Operator: QM
Sample : E2837-05 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 15 18:24 2013 Quant Results File: HL071113.RES

Instrument :
HPLC_L
ClientSampleId :
BG500SS03A

Manual Integrations
APPROVED

QI
7/12/2013 11:16:50 AM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL071113.M
Title :
Last Update : Thu Jul 11 21:31:35 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.31	637954	160.165 ug/L m

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005549.D HL071113.M

Tue Jul 16 08:05:23 2013

RPT1

Quantitation Report

Data File : S:\HPCHEM1\HPLC_L\DATA\HL071113\HL005549.D Vial: 16
Acq On : 12-Jul-2013, 00:32 Operator: QM
Sample : E2837-05 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Jul 15 18:24 2013 Quant Results File: HL071113.RES


Instrument :
HPLC_L
ClientSampleId :
BG500SS03A


Manual Integrations
APPROVED

QI
7/12/2013 11:16:50 AM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL071113.M
Title :
Last Update : Thu Jul 11 21:31:35 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

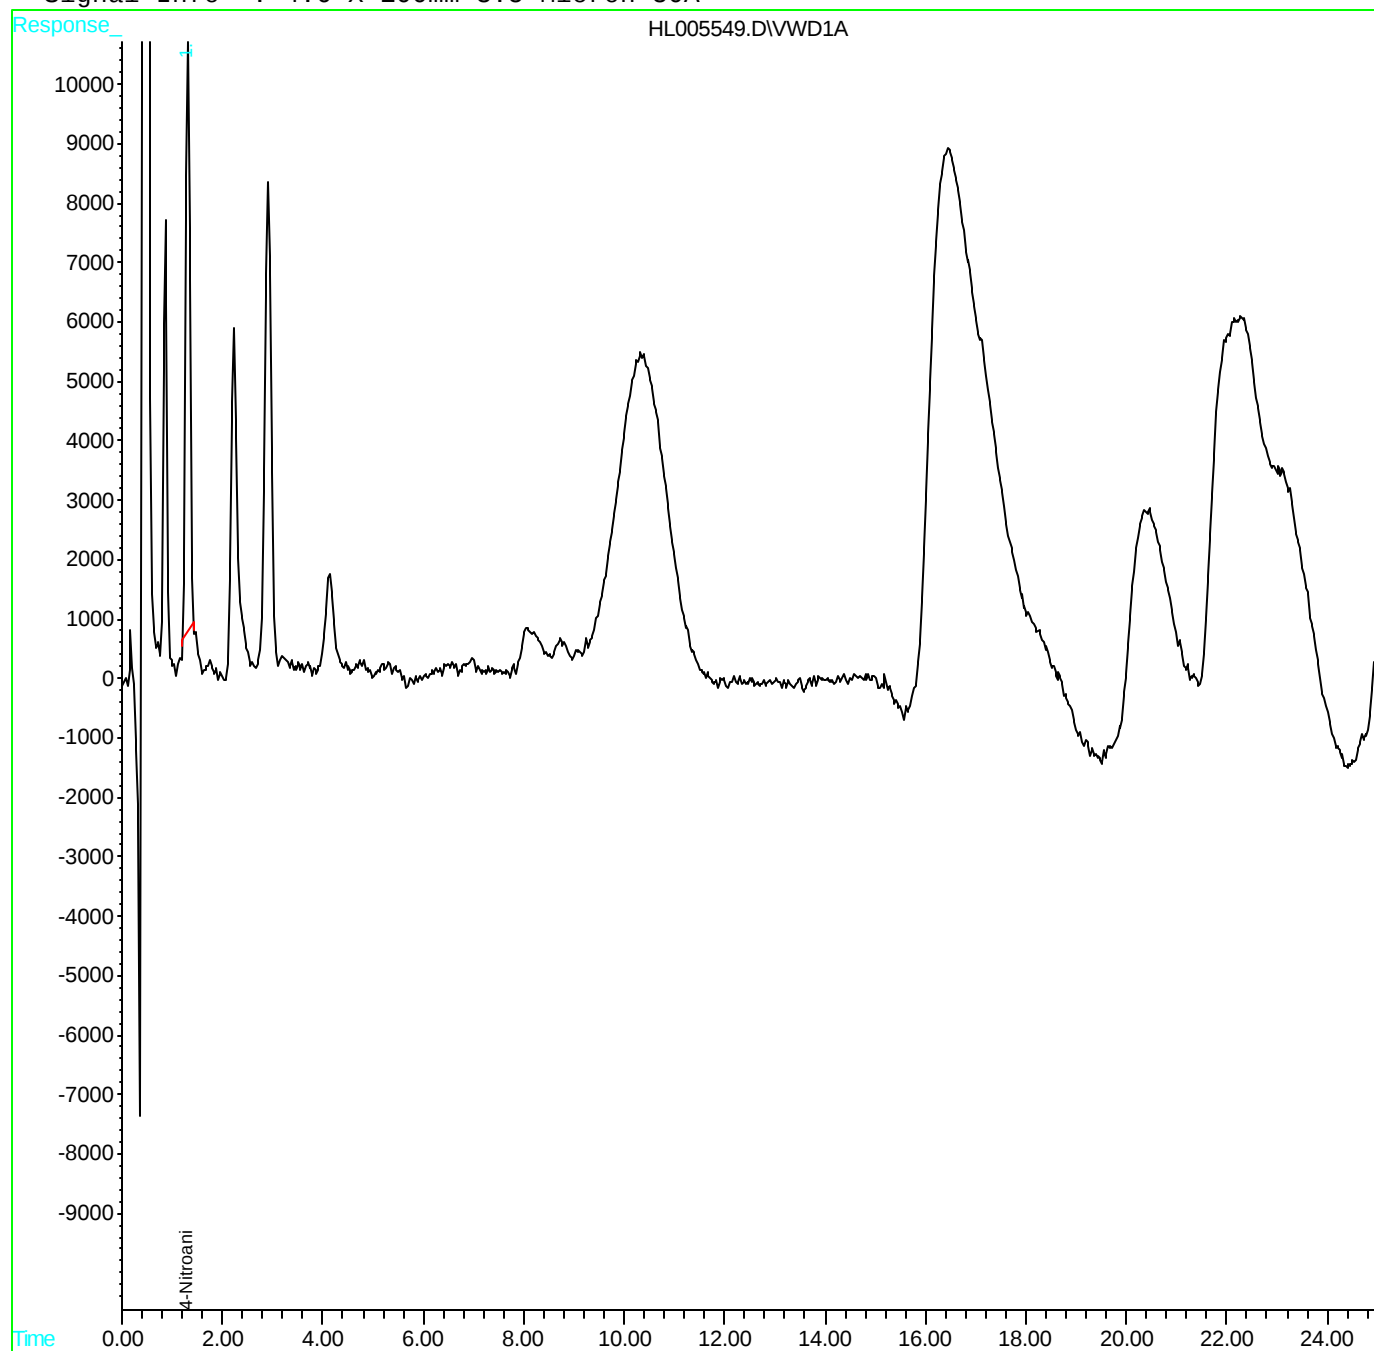

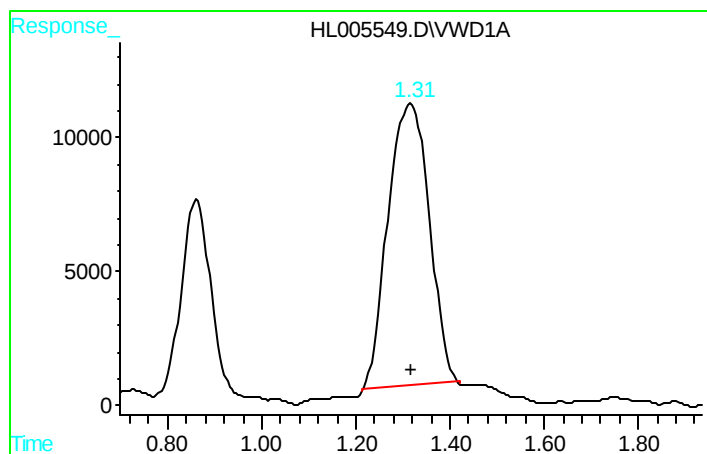

#1 4-Nitroaniline

R.T.: 1.314 min
Delta R.T.: -0.004 min
Response: 637954
Conc: 160.17 ug/L m

Instrument :
HPLC_L
ClientSampleId :
BG500SS03A

Manual Integrations
APPROVED

QI
7/12/2013 11:16:50 AM