

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL080215\
 Data File : HL006267.D
 Signal(s) : vwd1A.ch
 Acq On : 02-Aug-2015, 13:27
 Operator : TP/IZ
 Sample : SSTDICC2000
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 SSTDICC2000

Integration File: AUTOINT1.E
 Quant Time: Aug 04 02:27:39 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL080215.M
 Quant Title :
 QLast Update : Tue Aug 04 02:23:22 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) T HMX	1.257	10276075	1348.249 ug/L
3) T RDX	2.179	22862166	1609.600 ug/L
4) T 1,3,5-Trinitrobenzene	3.509	26506716	1368.735 ug/L
5) T 1,3-Dinitrobenzene	4.632	39885067	1382.386 ng/ml
6) T 3,5-Dinitroaniline	5.326	29498912	1338.871 ug/L
7) T Nitrobenzene	5.978	23421471	1404.864 ug/L
8) T Tetryl	7.901	16926882	1284.077 ug/L
9) T 2,4,6-Trinitrotoluene	8.377	24827578	1243.164 ug/L
10) T 2-Amino-4,6-dinitroto...	9.489	25968382	1266.550 ug/L
11) T 4-Amino-2,6-dinitroto...	9.979	16928510	1298.222 ug/L
12) T 2,4-Dinitrotoluene	10.720	37878363	1396.343 ug/L
13) T 2,6-Dinitrotoluene	11.048	18097161	1354.408 ug/L
14) T 2-Nitrotoluene	14.950	43465862	1393.306 ug/L
15) T 4-Nitrotoluene	16.244	35070071	1355.935 ug/L
16) T 3-Nitrotoluene	17.595	48236620	1370.745 ug/L
17) T PETN	18.650	23718953	1447.560 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL080215\
Data File : HL006267.D
Signal(s) : vwd1A.ch
Acq On : 02-Aug-2015, 13:27
Operator : TP/IZ
Sample : SSTDICC2000
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

Integration File: AUTOINT1.E
Quant Time: Aug 04 02:27:39 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL080215.M
Quant Title :
QLast Update : Tue Aug 04 02:23:22 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

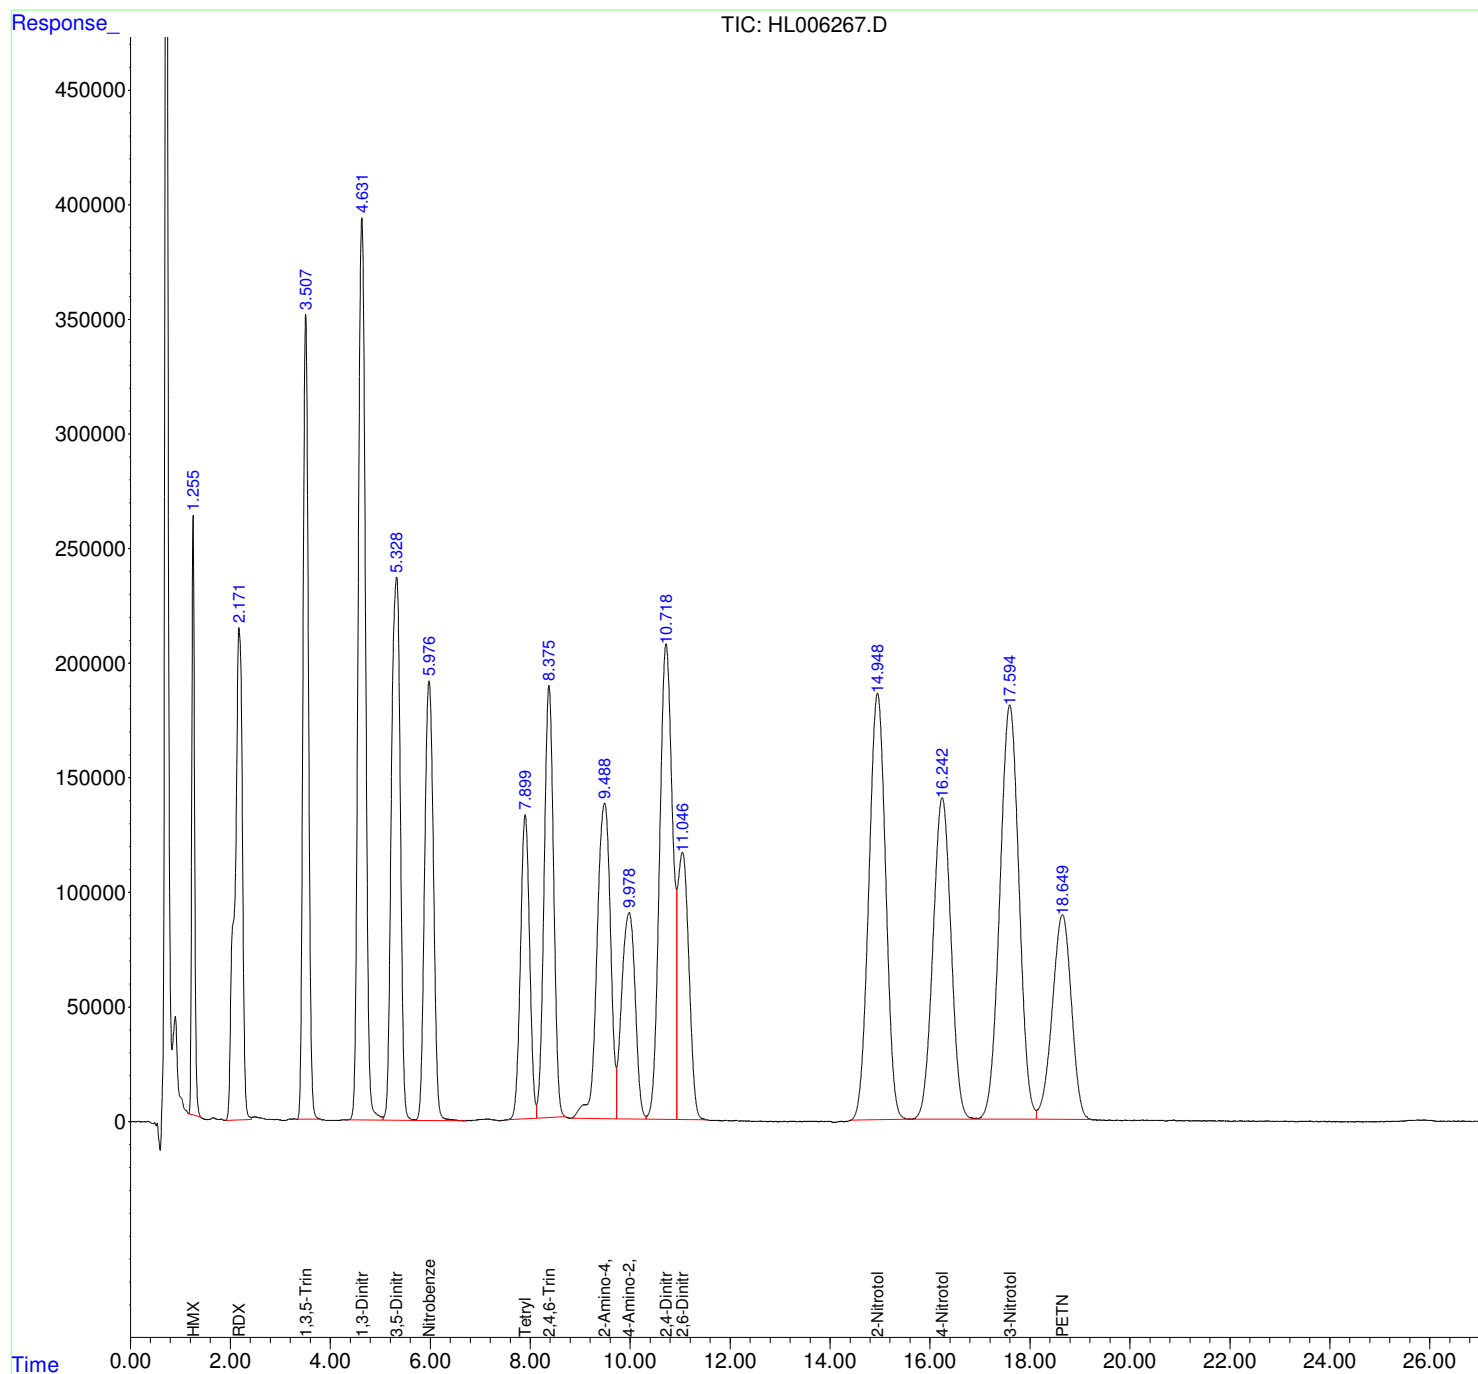


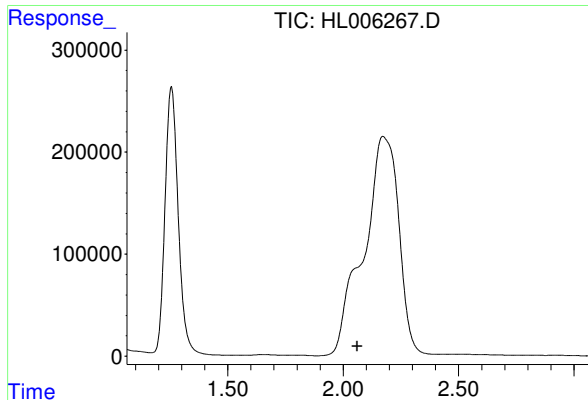

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 2.061 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

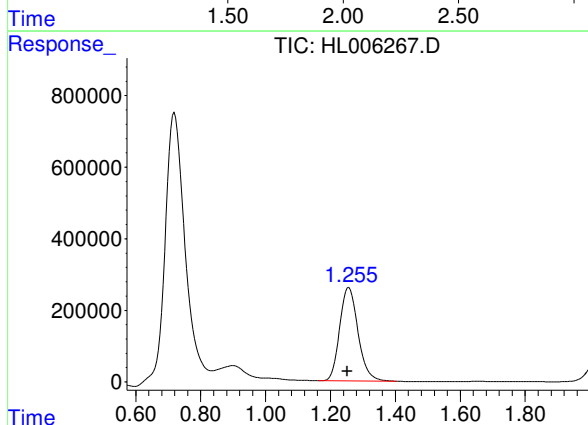


#2 HMX

R.T.: 1.257 min
Delta R.T.: 0.006 min
Response: 10276075
Conc: 1348.25 ug/L

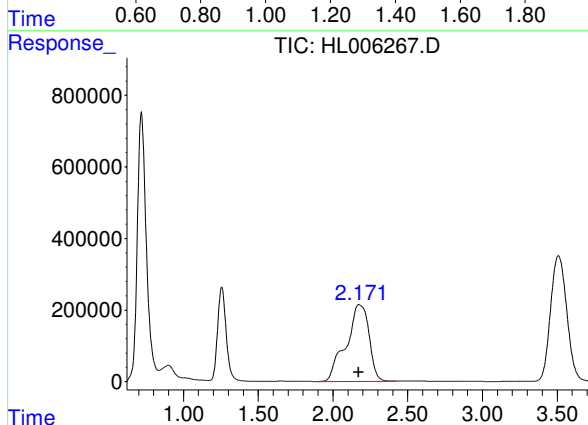


#3 RDX

R.T.: 2.179 min
Delta R.T.: 0.008 min
Response: 22862166
Conc: 1609.60 ug/L

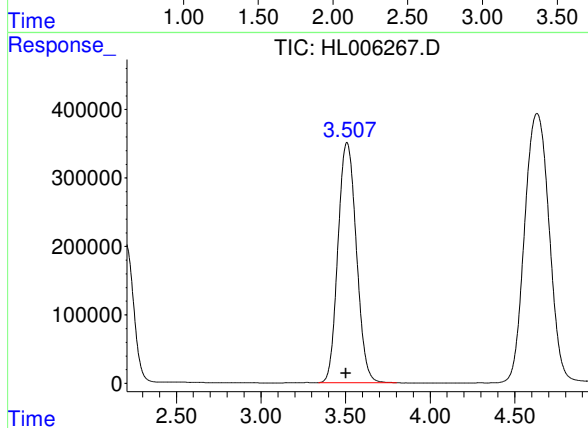

#4 1,3,5-Trinitrobenzene


R.T.: 3.509 min
Delta R.T.: 0.007 min
Response: 26506716
Conc: 1368.73 ug/L

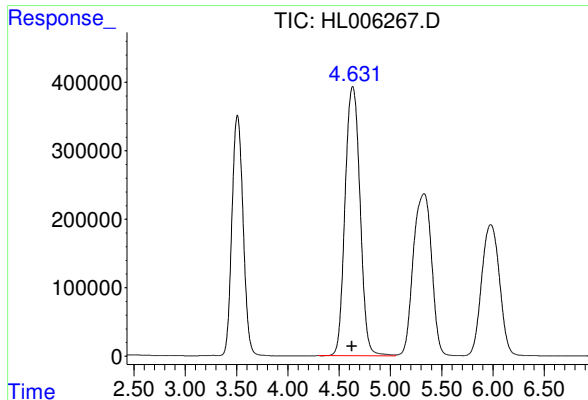

#5 1,3-Dinitrobenzene


R.T.: 4.632 min
Delta R.T.: 0.008 min
Response: 39885067
Conc: 1382.39 ng/ml

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

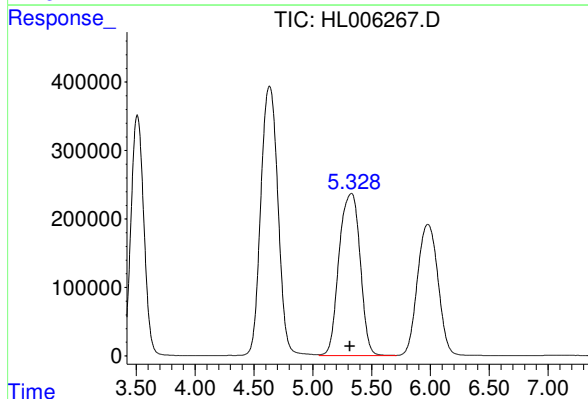


#6 3,5-Dinitroaniline

R.T.: 5.326 min
Delta R.T.: 0.009 min
Response: 29498912
Conc: 1338.87 ug/L

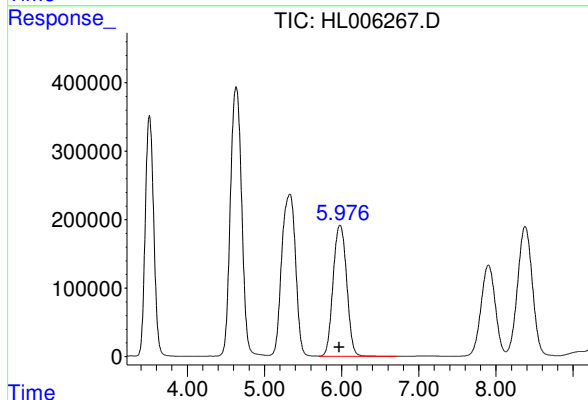


#7 Nitrobenzene

R.T.: 5.978 min
Delta R.T.: 0.009 min
Response: 23421471
Conc: 1404.86 ug/L

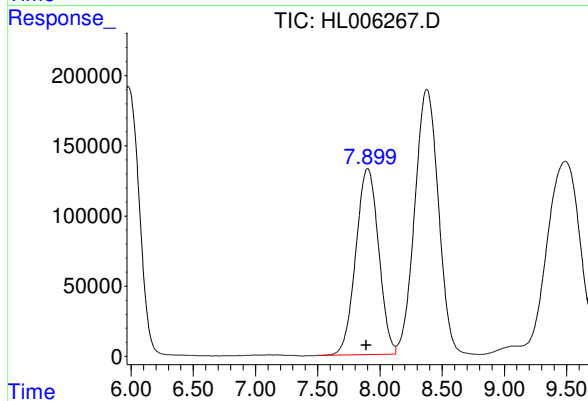

#8 Tetryl


R.T.: 7.901 min
Delta R.T.: 0.010 min
Response: 16926882
Conc: 1284.08 ug/L

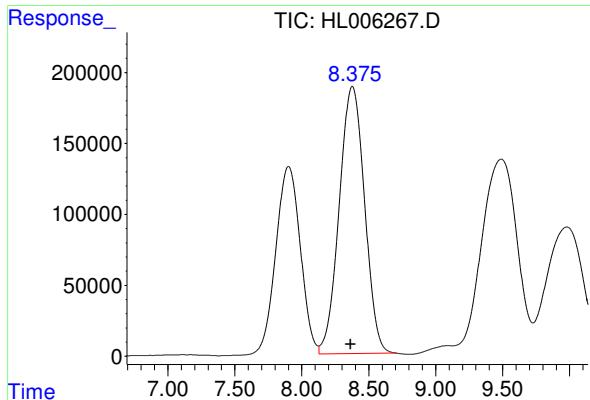

#9 2,4,6-Trinitrotoluene


R.T.: 8.377 min
Delta R.T.: 0.012 min
Response: 24827578
Conc: 1243.16 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

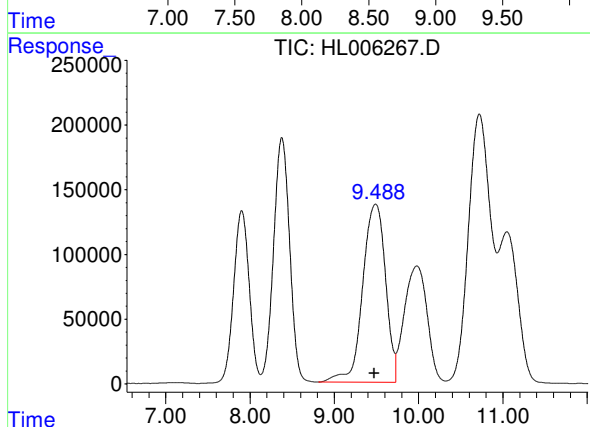


#10 2-Amino-4,6-dinitrotoluene

R.T.: 9.489 min
Delta R.T.: 0.014 min
Response: 25968382
Conc: 1266.55 ug/L

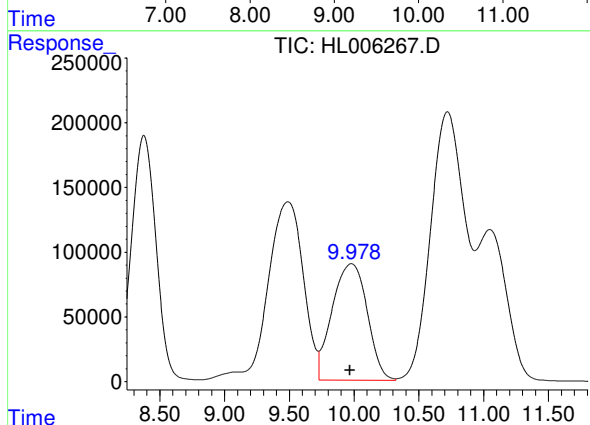


#11 4-Amino-2,6-dinitrotoluene

R.T.: 9.979 min
Delta R.T.: 0.012 min
Response: 16928510
Conc: 1298.22 ug/L

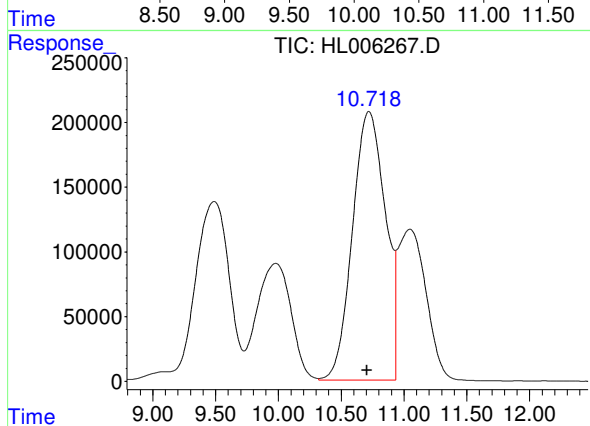

#12 2,4-Dinitrotoluene


R.T.: 10.720 min
Delta R.T.: 0.014 min
Response: 37878363
Conc: 1396.34 ug/L

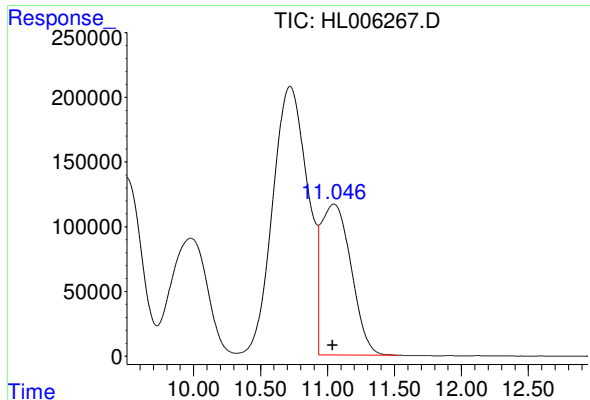

#13 2,6-Dinitrotoluene


R.T.: 11.048 min
Delta R.T.: 0.012 min
Response: 18097161
Conc: 1354.41 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000

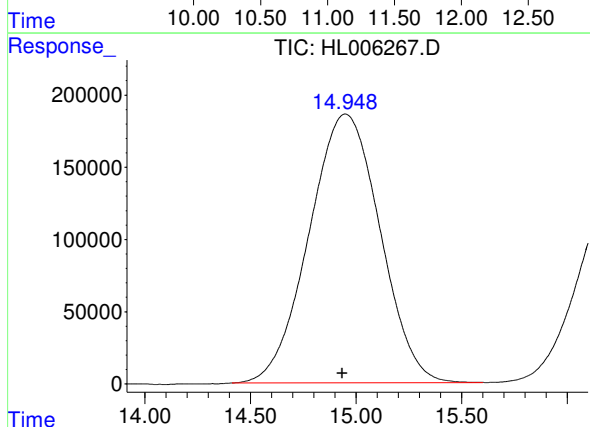


#14 2-Nitrotoluene

R.T.: 14.950 min
Delta R.T.: 0.014 min
Response: 43465862
Conc: 1393.31 ug/L

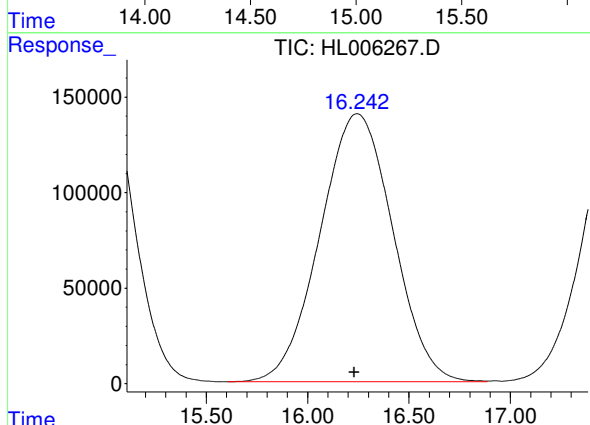


#15 4-Nitrotoluene

R.T.: 16.244 min
Delta R.T.: 0.015 min
Response: 35070071
Conc: 1355.94 ug/L

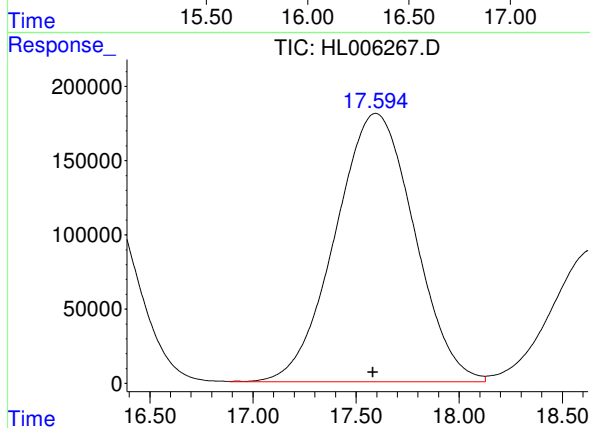

#16 3-Nitrotoluene

R.T.: 17.595 min
Delta R.T.: 0.016 min
Response: 48236620
Conc: 1370.74 ug/L

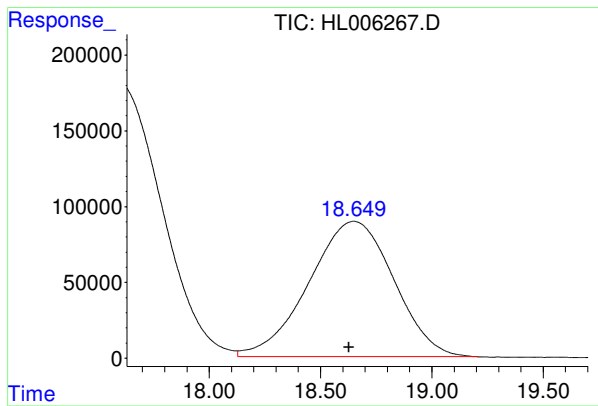

#17 PETN

R.T.: 18.650 min
Delta R.T.: 0.023 min
Response: 23718953
Conc: 1447.56 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICC2000