

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL080215\
 Data File : HL006273.D
 Signal(s) : vwd1A.ch
 Acq On : 02-Aug-2015, 16:17
 Operator : TP/IZ
 Sample : SSTDICV0500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 SSTDICV0500

Integration File: AUTOINT1.E
 Quant Time: Aug 11 18:12:12 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL080215.M
 Quant Title :
 QLast Update : Tue Aug 04 03:05:03 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) T HMX	1.257	2808088	430.912 ug/L
3) T RDX	2.185	6235086	512.882 ug/L
4) T 1,3,5-Trinitrobenzene	3.506	7433965	434.152 ug/L
5) T 1,3-Dinitrobenzene	4.627	11001216	431.752 ng/ml
6) T 3,5-Dinitroaniline	5.314	8096992	429.547 ug/L
7) T Nitrobenzene	5.971	6338783	425.419 ug/L
8) T Tetryl	7.891	5306605	451.131 ug/L
9) T 2,4,6-Trinitrotoluene	8.367	6918714	435.307 ug/L
10) T 2-Amino-4,6-dinitroto...	9.475	7058993	427.658 ug/L
11) T 4-Amino-2,6-dinitroto...	9.961	4718328	429.500 ug/L
12) T 2,4-Dinitrotoluene	10.705	10189166	425.025 ug/L
13) T 2,6-Dinitrotoluene	11.034	5129017	436.919 ug/L
14) T 2-Nitrotoluene	14.929	11986670	429.812 ug/L
15) T 4-Nitrotoluene	16.222	9677245	429.724 ug/L
16) T 3-Nitrotoluene	17.571	13381718	431.181 ug/L
17) T PETN	18.618	6600635	432.005 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL080215\
Data File : HL006273.D
Signal(s) : vwd1A.ch
Acq On : 02-Aug-2015, 16:17
Operator : TP/IZ
Sample : SSTDICV0500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
SSTDICV0500

Integration File: AUTOINT1.E
Quant Time: Aug 11 18:12:12 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL080215.M
Quant Title :
QLast Update : Tue Aug 04 03:05:03 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

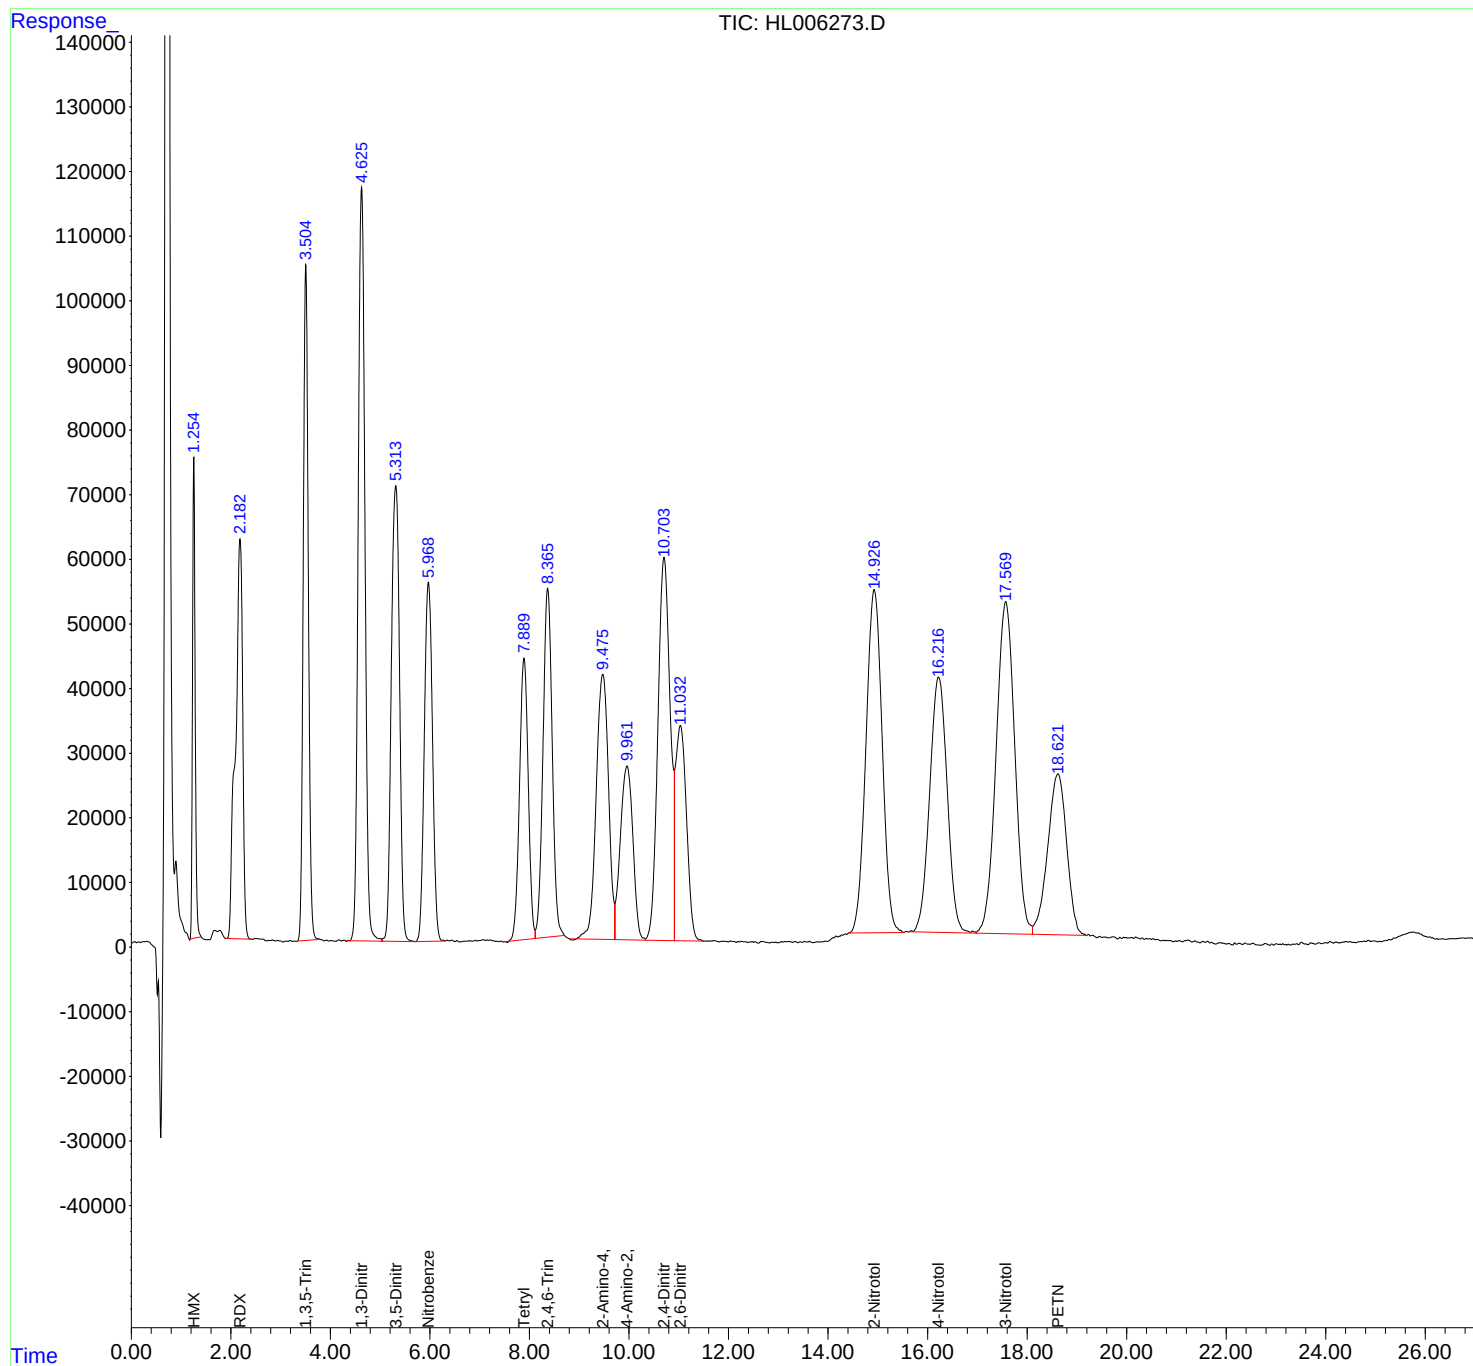


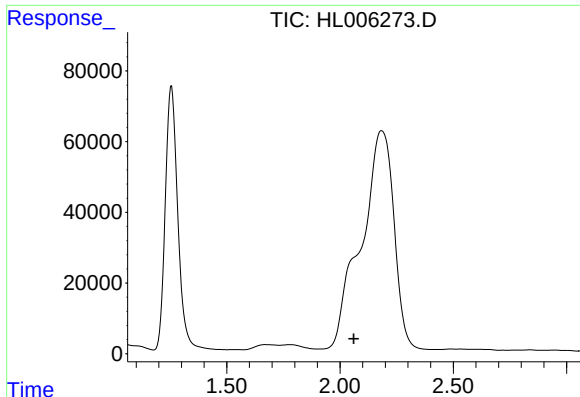

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 2.061 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
SSTDICV0500

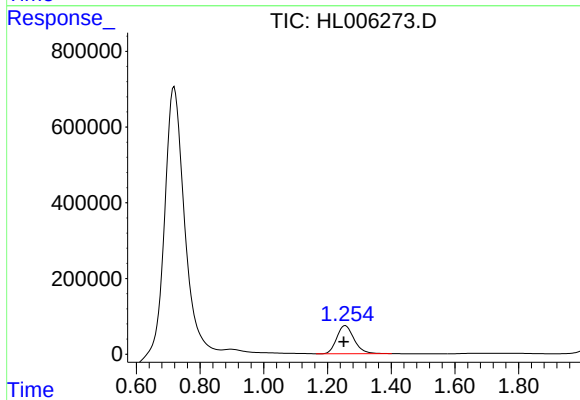


#2 HMX

R.T.: 1.257 min
Delta R.T.: 0.005 min
Response: 2808088
Conc: 430.91 ug/L

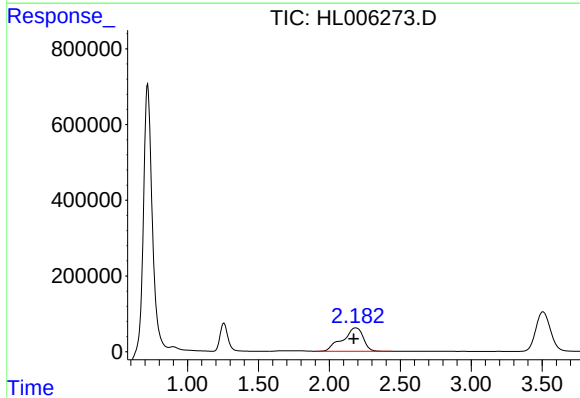


#3 RDX

R.T.: 2.185 min
Delta R.T.: 0.014 min
Response: 6235086
Conc: 512.88 ug/L

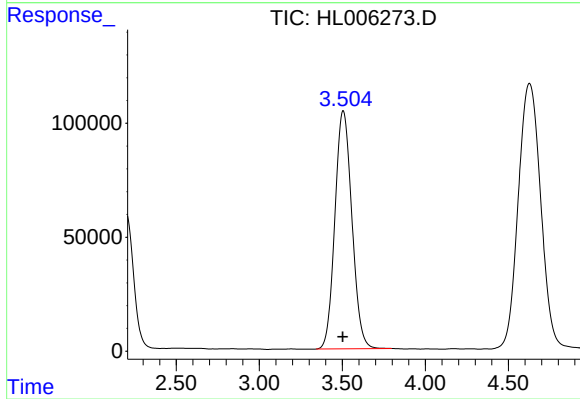

#4 1,3,5-Trinitrobenzene


R.T.: 3.506 min
Delta R.T.: 0.004 min
Response: 7433965
Conc: 434.15 ug/L

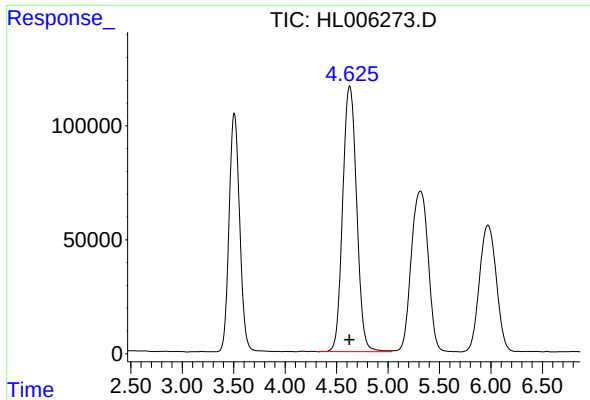

#5 1,3-Dinitrobenzene


R.T.: 4.627 min
Delta R.T.: 0.003 min
Response: 11001216
Conc: 431.75 ng/ml

Instrument :
HPLC_L
ClientSampleId :
SSTDICV0500

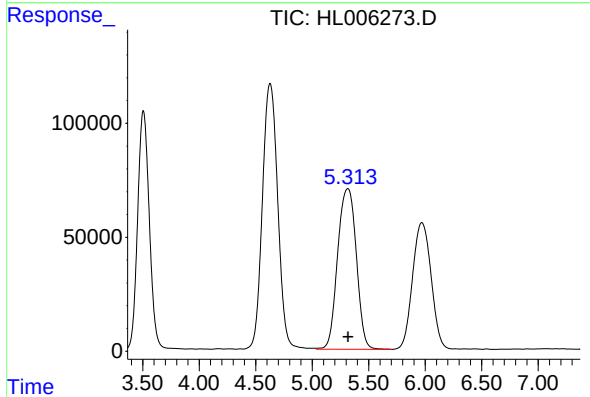


#6 3,5-Dinitroaniline

R.T.: 5.314 min
Delta R.T.: -0.003 min
Response: 8096992
Conc: 429.55 ug/L

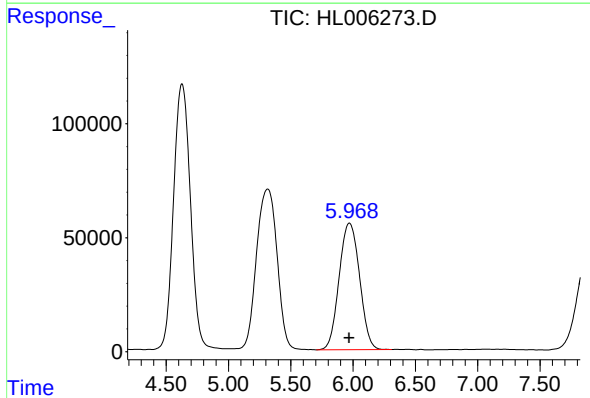


#7 Nitrobenzene

R.T.: 5.971 min
Delta R.T.: 0.002 min
Response: 6338783
Conc: 425.42 ug/L

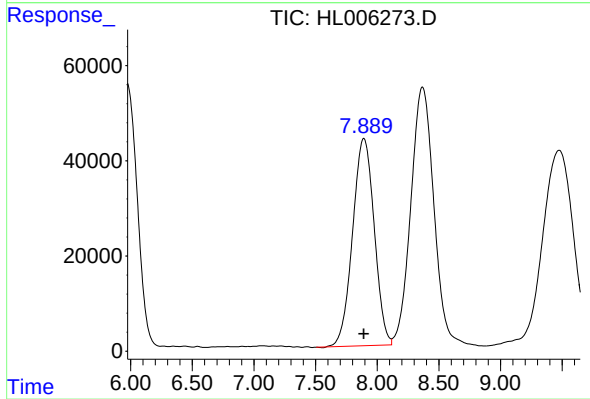

#8 Tetryl


R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 5306605
Conc: 451.13 ug/L

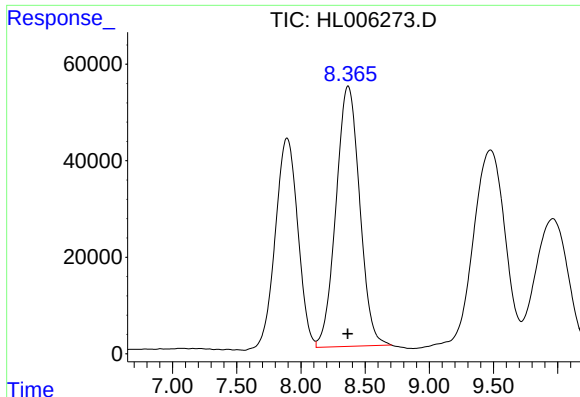

#9 2,4,6-Trinitrotoluene


R.T.: 8.367 min
Delta R.T.: 0.002 min
Response: 6918714
Conc: 435.31 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICV0500

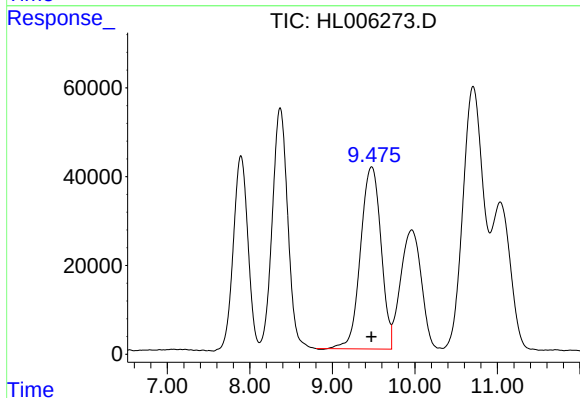


#10 2-Amino-4,6-dinitrotoluene

R.T.: 9.475 min
Delta R.T.: 0.000 min
Response: 7058993
Conc: 427.66 ug/L

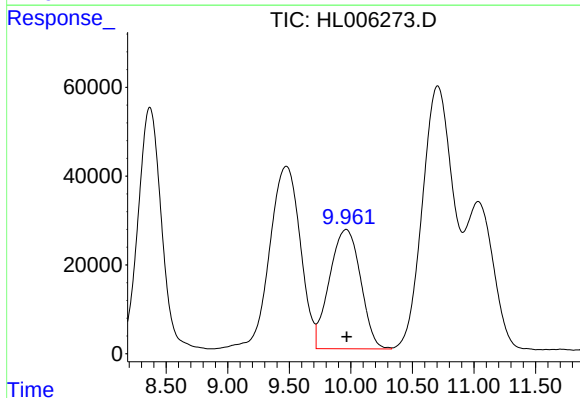


#11 4-Amino-2,6-dinitrotoluene

R.T.: 9.961 min
Delta R.T.: -0.006 min
Response: 4718328
Conc: 429.50 ug/L

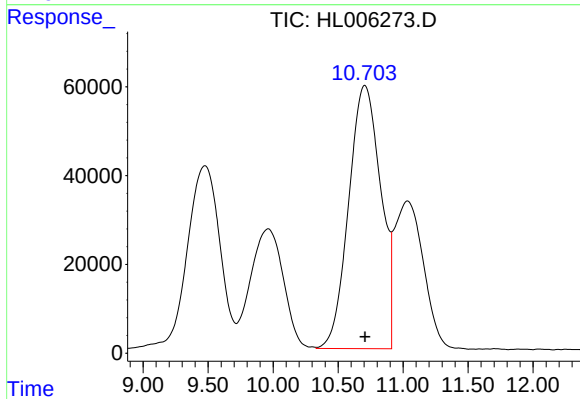

#12 2,4-Dinitrotoluene


R.T.: 10.705 min
Delta R.T.: -0.001 min
Response: 10189166
Conc: 425.02 ug/L

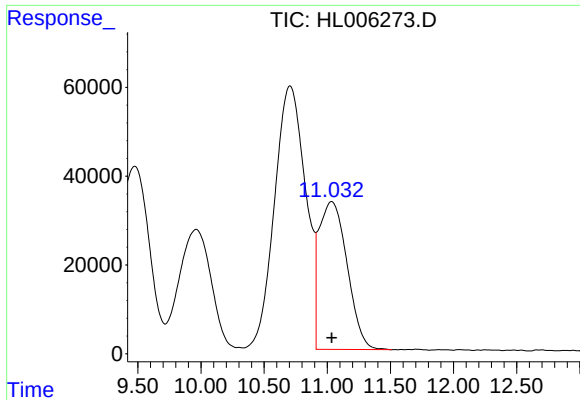

#13 2,6-Dinitrotoluene


R.T.: 11.034 min
Delta R.T.: -0.002 min
Response: 5129017
Conc: 436.92 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICV0500

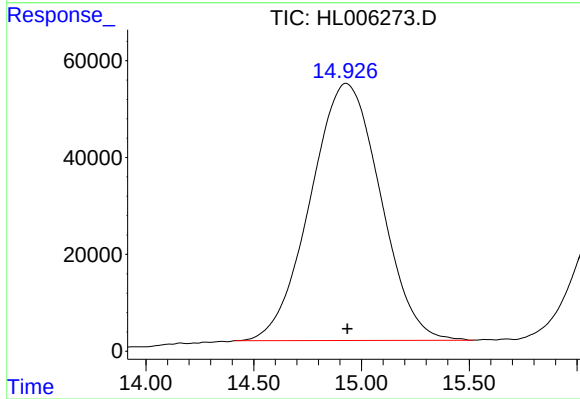


#14 2-Nitrotoluene

R.T.: 14.929 min
Delta R.T.: -0.007 min
Response: 11986670
Conc: 429.81 ug/L

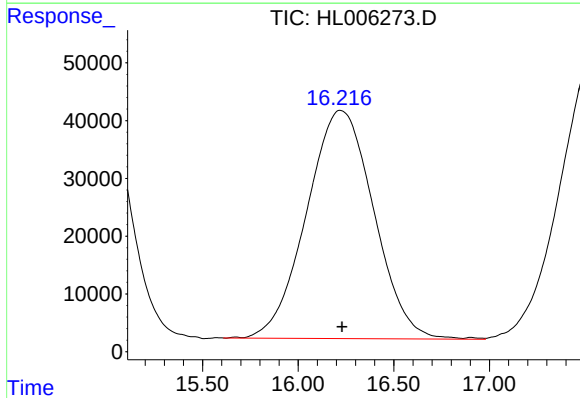


#15 4-Nitrotoluene

R.T.: 16.222 min
Delta R.T.: -0.008 min
Response: 9677245
Conc: 429.72 ug/L

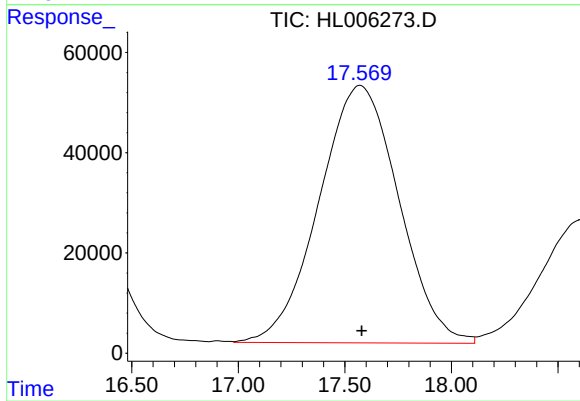

#16 3-Nitrotoluene

R.T.: 17.571 min
Delta R.T.: -0.009 min
Response: 13381718
Conc: 431.18 ug/L

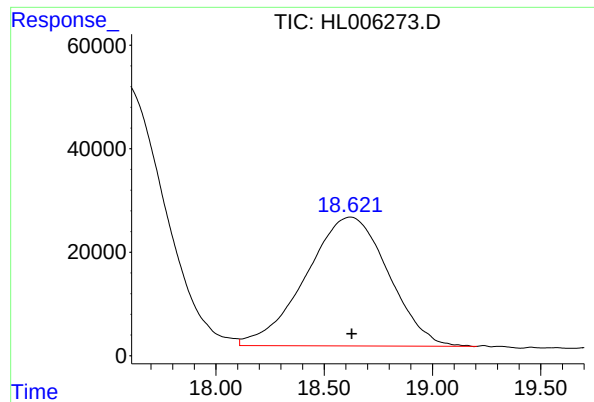

#17 PETN

R.T.: 18.618 min
Delta R.T.: -0.008 min
Response: 6600635
Conc: 432.01 ug/L

Instrument :
HPLC_L
ClientSampleId :
SSTDICV0500