

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL080215\
Data File : HL006281.D
Signal(s) : vwd1A.ch
Acq On : 02-Aug-2015, 20:05
Operator : TP/IZ
Sample : SSTDICC010
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
SSTDICC010

Integration File: AUTOINT1.E
Quant Time: Aug 04 03:21:47 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL0802NG.M
Quant Title :
QLast Update : Tue Aug 04 03:21:40 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.110	48532775	9.233 ng/ul
Target Compounds			
2) T Nitroglycerin	6.590	105732826	9.610 ng/ul

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL080215\
Data File : HL006281.D
Signal(s) : vwd1A.ch
Acq On : 02-Aug-2015, 20:05
Operator : TP/IZ
Sample : SSTDICC010
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
SSTDICC010

Integration File: AUTOINT1.E
Quant Time: Aug 04 03:21:47 2015
Quant Method : Z:\HPCHEM1\HPLC_L\Methods\HL0802NG.M
Quant Title :
QLast Update : Tue Aug 04 03:21:40 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

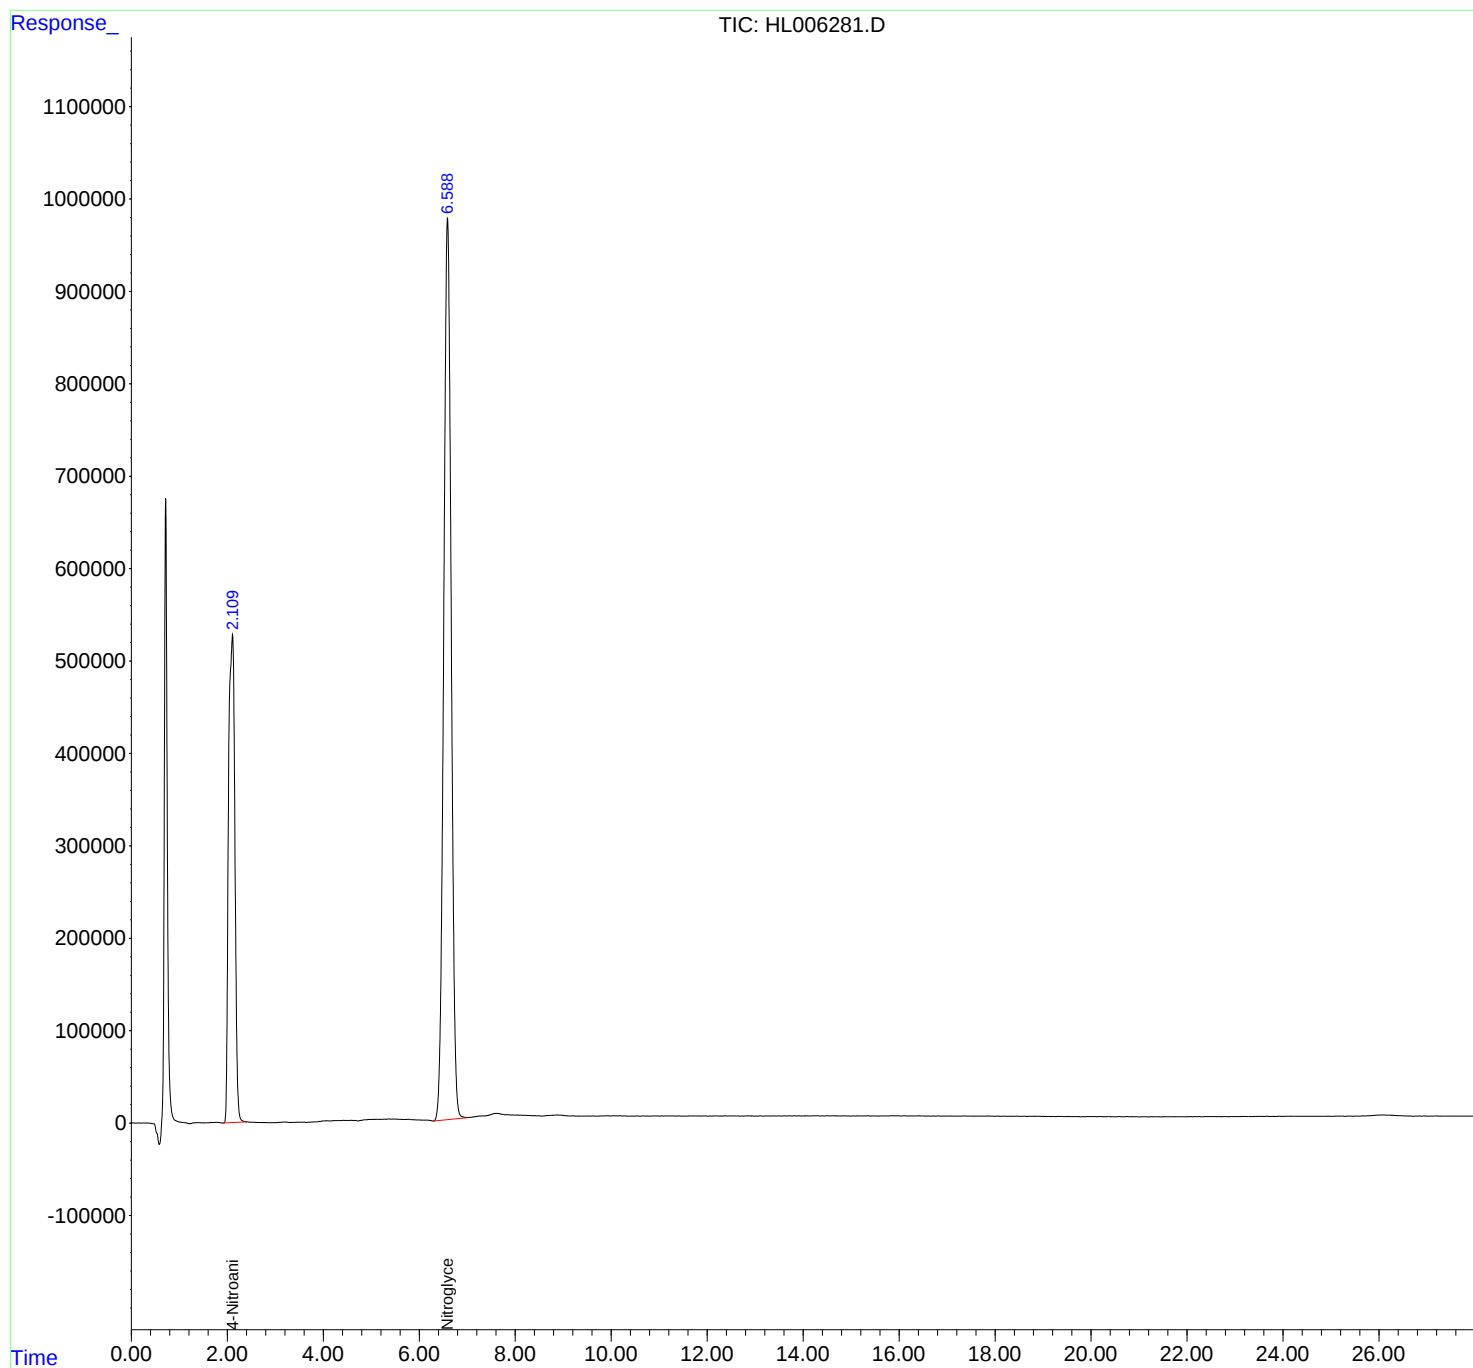


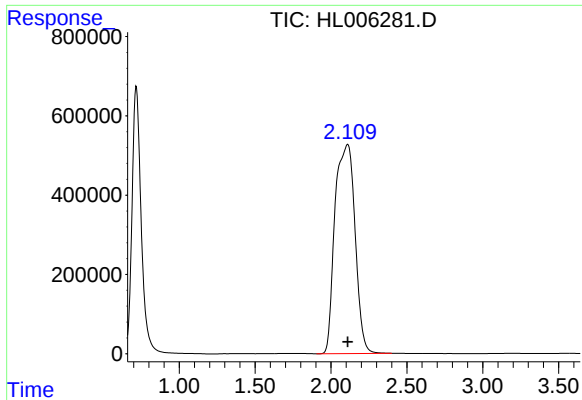

#1 4-Nitroaniline

R.T.: 2.110 min
Delta R.T.: 0.000 min
Response: 48532775
Conc: 9.23 ng/ul

Instrument :
HPLC_L
ClientSampleId :
SSTDIC010

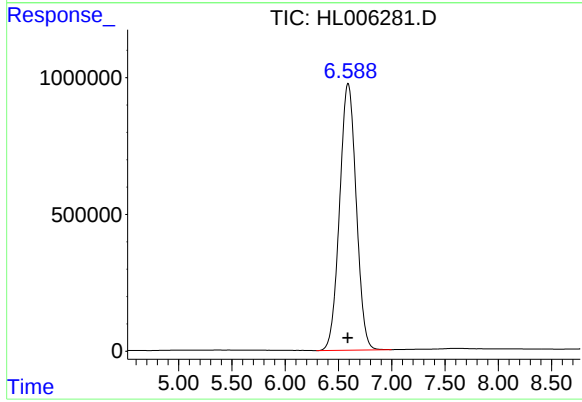

#2 Nitroglycerin

R.T.: 6.590 min
Delta R.T.: 0.002 min
Response: 105732826
Conc: 9.61 ng/ul