

Data File : H:\VOL1\HPLC\HPLC L\120821\HL003410.D Vial: 28
Acq On : 21-Aug-2012, 15:52 Operator: HLM
Sample : D3778-01MSD2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Aug 23 16:30 2012 Quant Results File: HL080312.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL080312.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Thu Aug 23 16:30:31 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.37	654509	178.456 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 59.49%

Target Compounds


5) T	Tetryl	6.25f	137238	15.887 ug/L
6) T	2,4,6-Trinitrotoluene	6.69	8069485	734.404 ug/L
17) T	Nitroglycerin	6.25	137238	2400.595 ug/L
18) T	PETN	19.31	846931	86.330 ug/L


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\120821\HL003410.D Vial: 28
 Acq On : 21-Aug-2012, 15:52 Operator: HLM
 Sample : D3778-01MSD2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Aug 23 16:30 2012 Quant Results File: HL080312.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL080312.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Thu Aug 23 16:30:31 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M


Volume Inj. :
 Signal Phase :
 Signal Info :

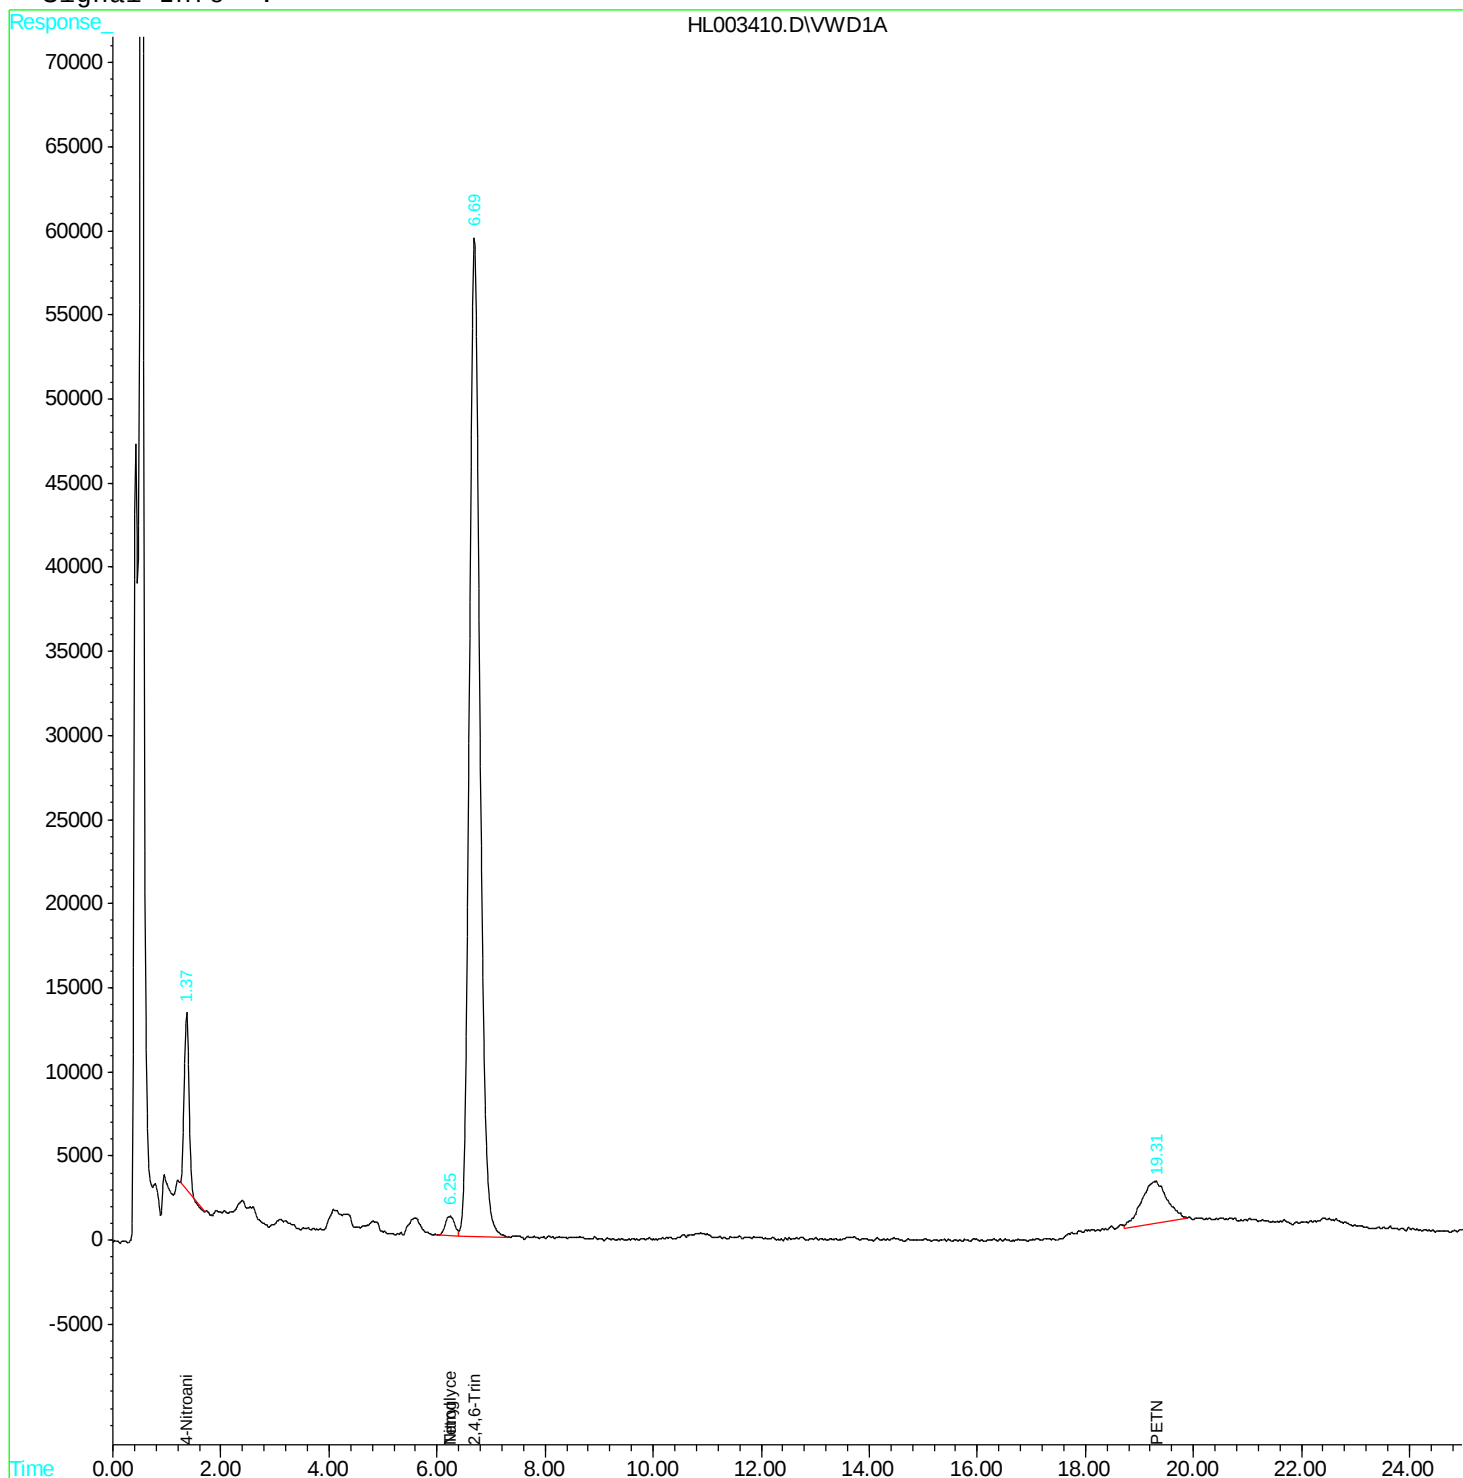

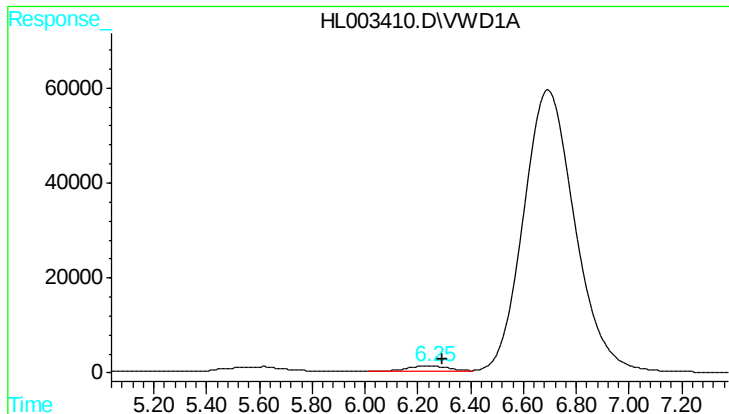


#5 Tetryl

R.T.: 6.247 min
 Delta R.T.: -0.047 min
 Response: 137238
 Conc: 15.89 ug/L

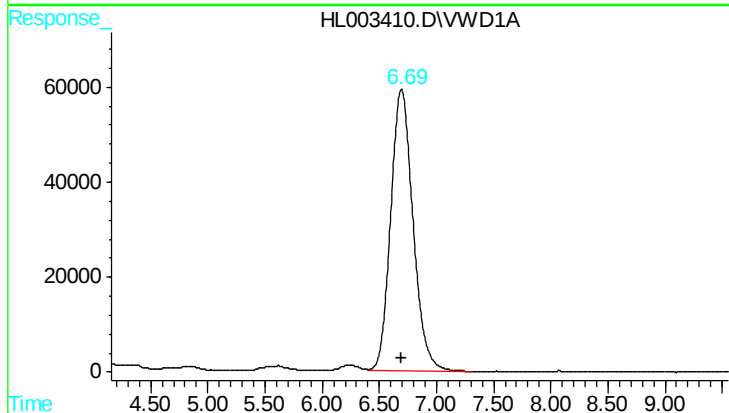


#6 2,4,6-Trinitrotoluene

R.T.: 6.694 min
 Delta R.T.: 0.004 min
 Response: 8069485
 Conc: 734.40 ug/L

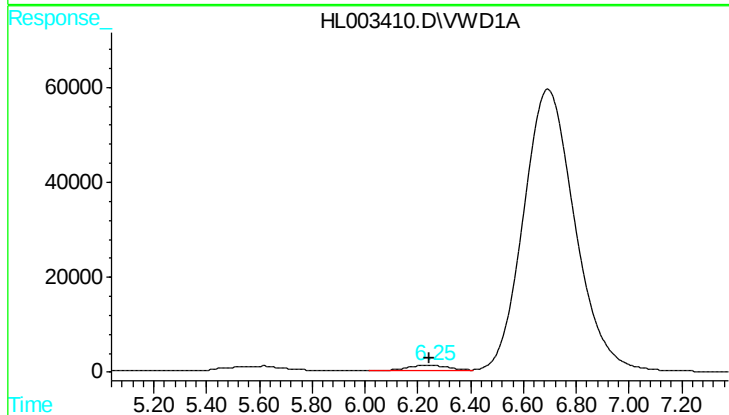

#17 Nitroglycerin

R.T.: 6.247 min
 Delta R.T.: 0.004 min
 Response: 137238
 Conc: 2400.60 ug/L

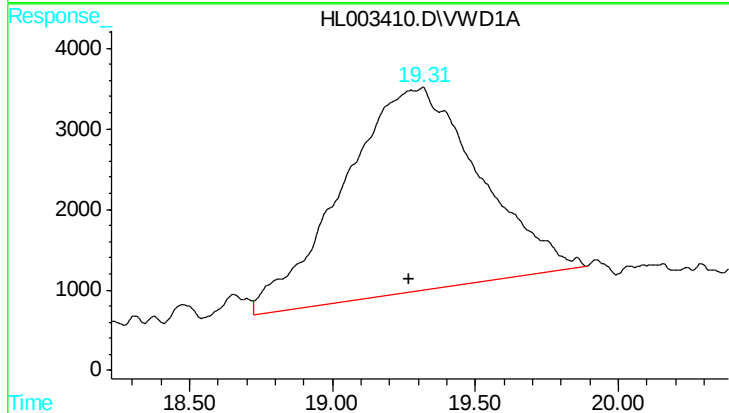

#18 PETN

R.T.: 19.314 min
 Delta R.T.: 0.048 min
 Response: 846931
 Conc: 86.33 ug/L