

Data File : H:\VOL1\HPLC\HPLC L\120919\HL003465.D Vial: 8
 Acq On : 19-Sep-2012, 15:40 Operator: HLM
 Sample : 8330-ICV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Sep 20 8:29 2012 Quant Results File: HL091912.RES

Instrument :
 HPLC_L
 ClientSampleId :
 ICVHL091912

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Thu Sep 20 08:25:48 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) T HMX	0.90	3986103	1018.959 ug/L
3) T RDX	1.72	5422894	1042.827 ug/L
4) T 1,3,5-Trinitrobenzene	2.68	11955725	984.794 ug/L
5) T Tetrvl	6.00	8668448	1015.642 ug/L
6) T 2,4,6-Trinitrotoluene	6.41	11559836	1025.901 ug/L
7) T 2-Amino-4,6-dinitrotoluene	6.83	10793070	991.503 ug/L
8) T 4-Amino-2,6-dinitrotoluene	7.13	7387679	1069.044 ug/L
9) T 2,4-Dinitrotoluene	7.99	14496101	960.368 ug/L
10) T 2,6-Dinitrotoluene	8.35	8297636	953.293 ug/L
11) T 1,3-Dinitrobenzene	3.55	16037768	1012.316 ug/L
12) T Nitrobenzene	4.77	10267637	998.660 ug/L
13) T 2-Nitrotoluene	11.52	6586871	998.823 ug/L
14) T 3-Nitrotoluene	13.49	6999051	989.654 ug/L
15) T 4-Nitrotoluene	12.25	5594790	1013.579 ug/L
16) T 3,5-Dinitroaniline	3.87	13551587	886.073 ug/L
17) T Nitroglycerin	6.00	8668448	152638.956 ug/L
18) T PETN	18.32	8958669	925.954 ug/L

Data File : H:\VOL1\HPLC\HPLC L\120919\HL003465.D

Vial: 8

Acq On : 19-Sep-2012, 15:40

Operator: HLM

Sample : 8330-ICV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Sep 20 8:29 2012 Quant Results File: HL091912.RES

Instrument :

HPLC_L

ClientSampleId :

ICVHL091912

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Thu Sep 20 08:25:48 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

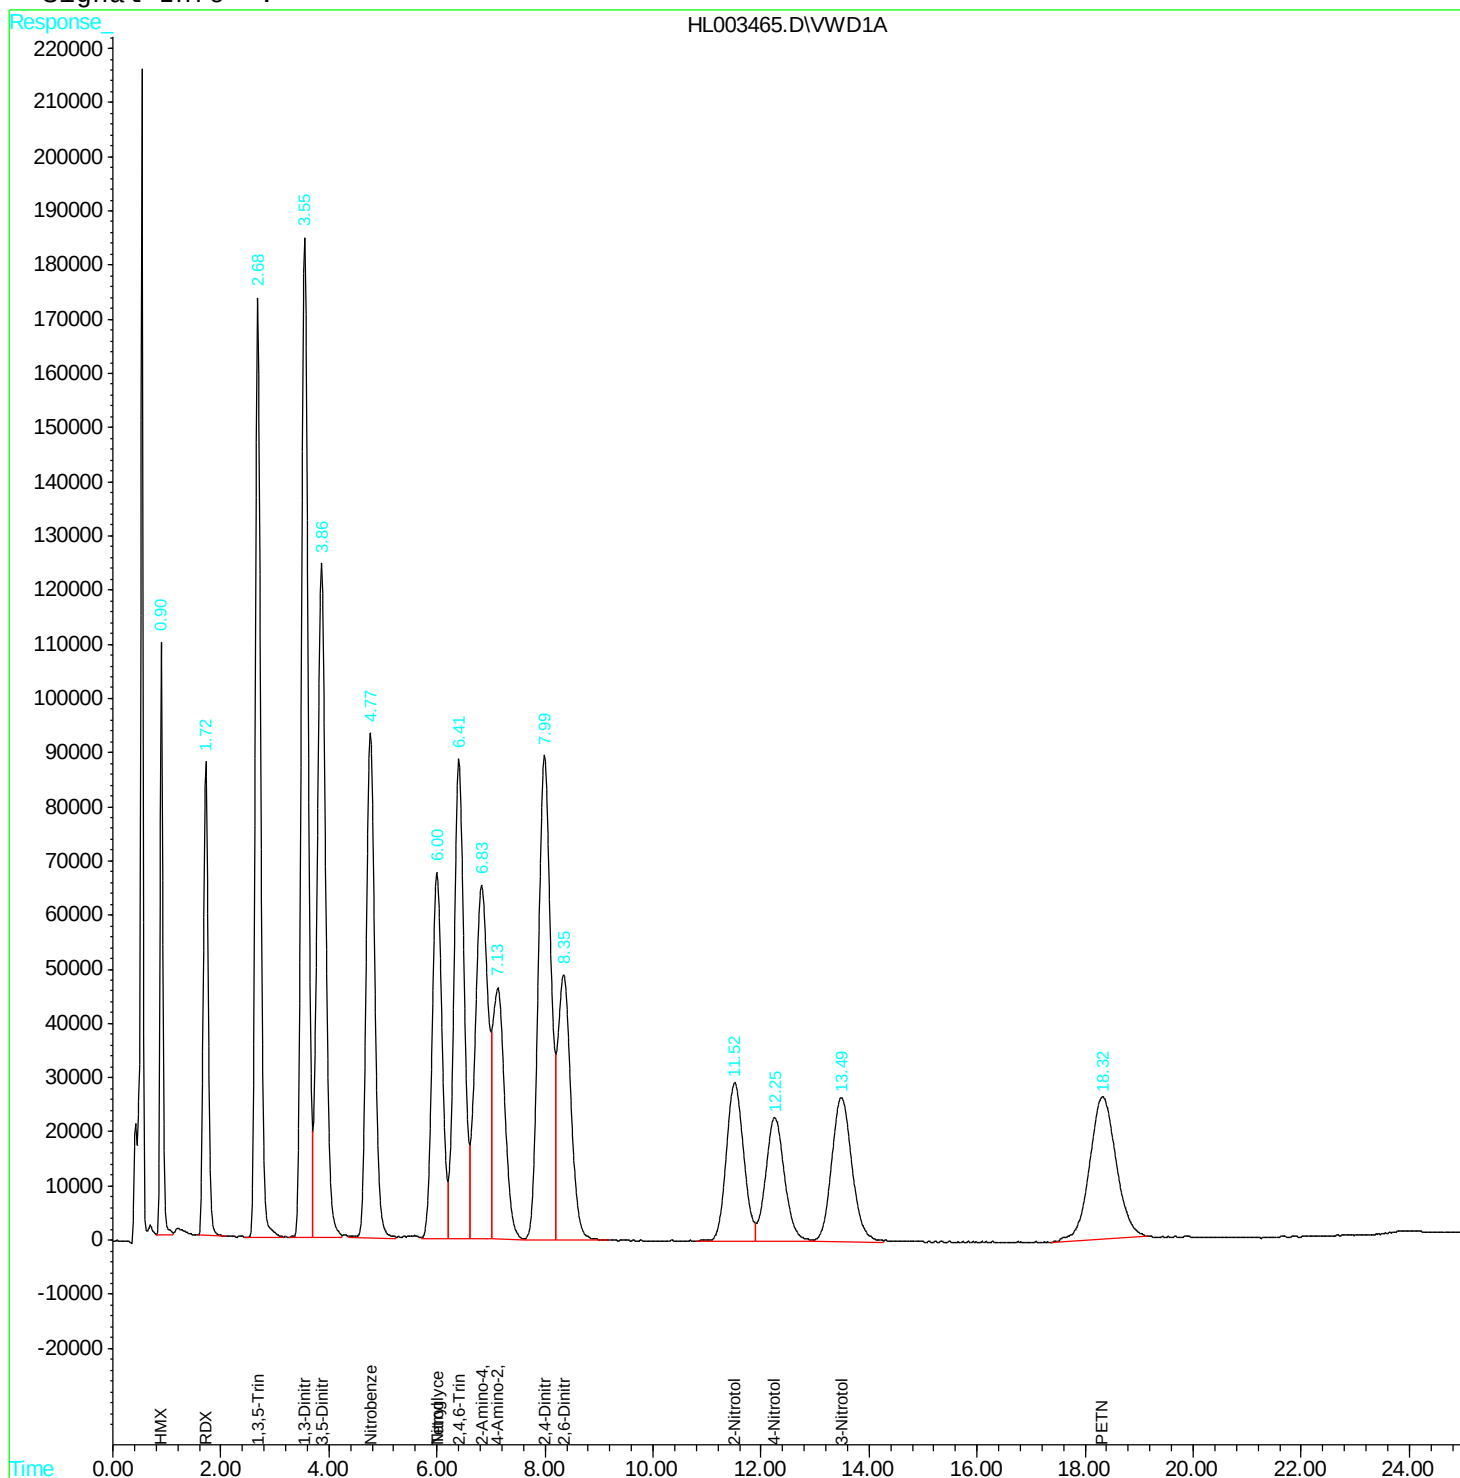


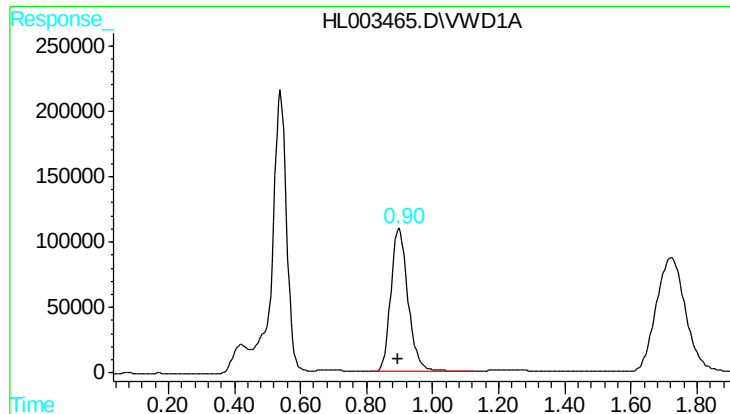

#2 HMX


R.T.: 0.899 min
Delta R.T.: 0.003 min
Response: 3986103
Conc: 1018.96 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL091912

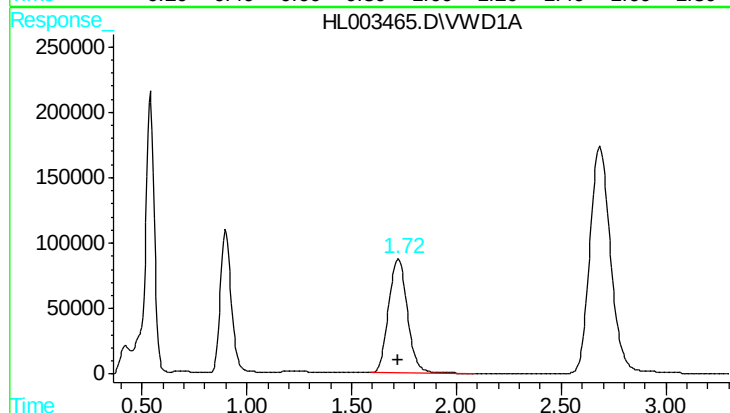


#3 RDX

R.T.: 1.723 min
Delta R.T.: 0.003 min
Response: 5422894
Conc: 1042.83 ug/L

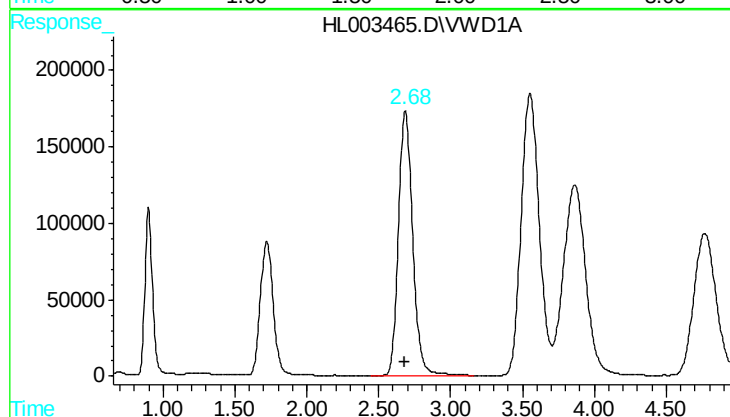


#4 1,3,5-Trinitrobenzene

R.T.: 2.685 min
Delta R.T.: 0.002 min
Response: 11955725
Conc: 984.79 ug/L

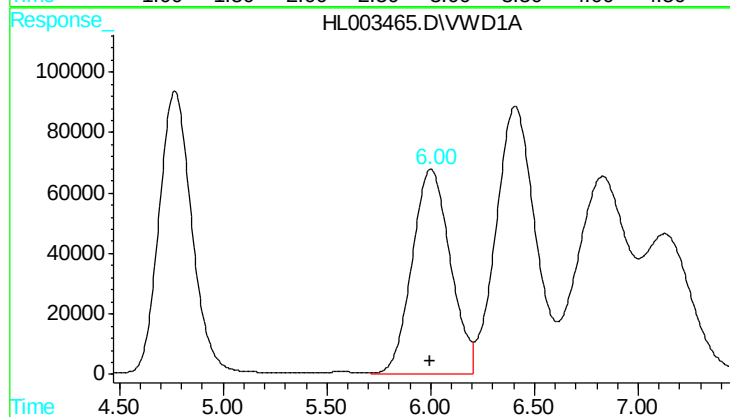

#5 Tetryl


R.T.: 6.002 min
Delta R.T.: 0.003 min
Response: 8668448
Conc: 1015.64 ug/L

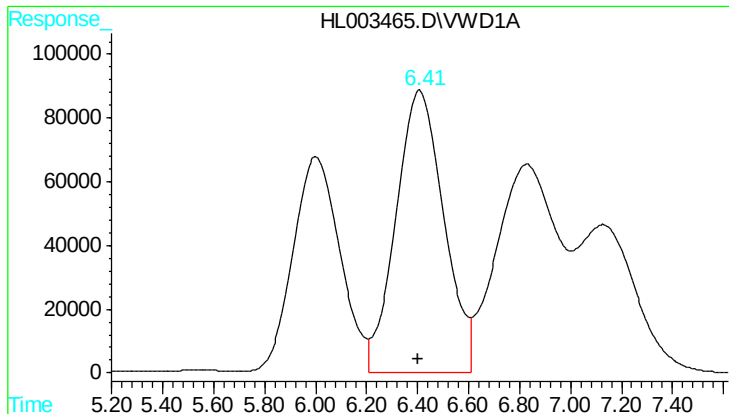

#6 2,4,6-Trinitrotoluene


R.T.: 6.408 min
Delta R.T.: 0.004 min
Response: 11559836
Conc: 1025.90 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL091912

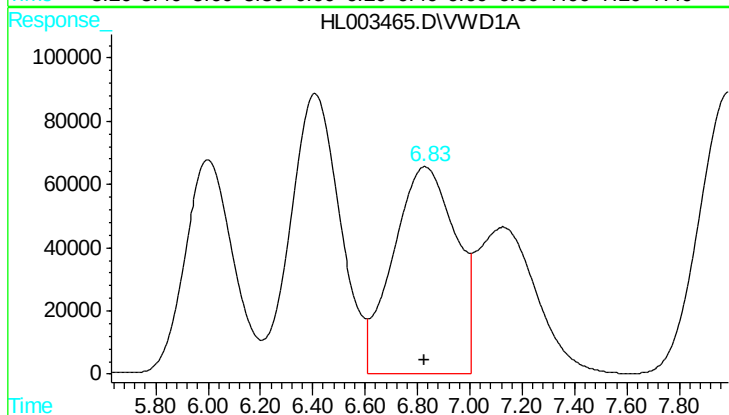


#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.829 min
Delta R.T.: 0.003 min
Response: 10793070
Conc: 991.50 ug/L

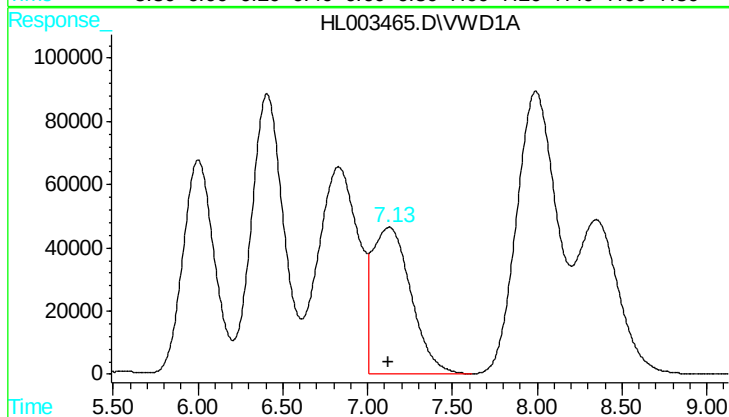


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.128 min
Delta R.T.: 0.002 min
Response: 7387679
Conc: 1069.04 ug/L

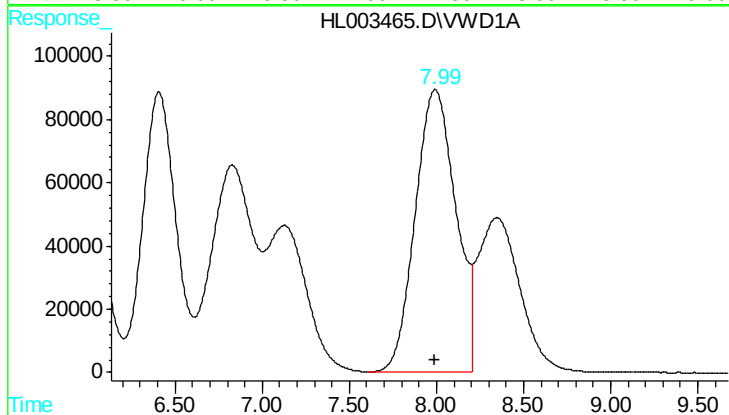

#9 2,4-Dinitrotoluene


R.T.: 7.992 min
Delta R.T.: 0.004 min
Response: 14496101
Conc: 960.37 ug/L

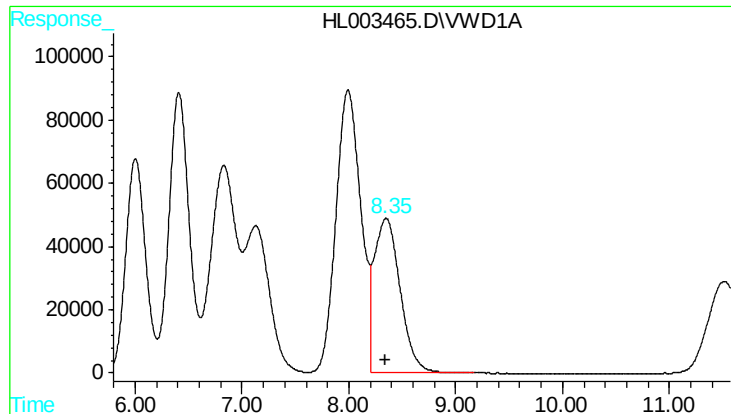

#10 2,6-Dinitrotoluene


R.T.: 8.348 min
Delta R.T.: 0.005 min
Response: 8297636
Conc: 953.29 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL091912

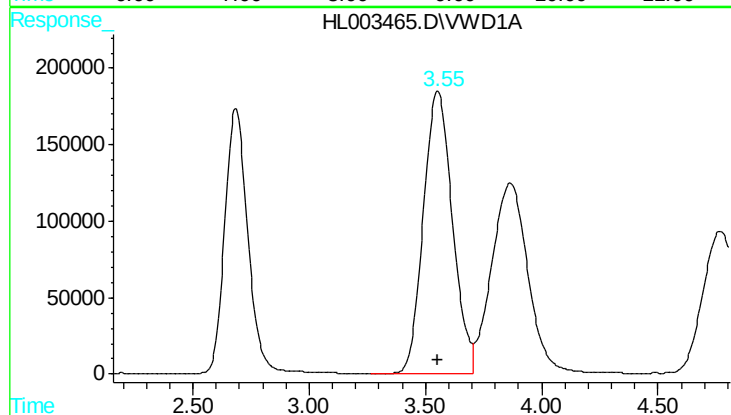


#11 1,3-Dinitrobenzene

R.T.: 3.553 min
Delta R.T.: 0.000 min
Response: 16037768
Conc: 1012.32 ug/L

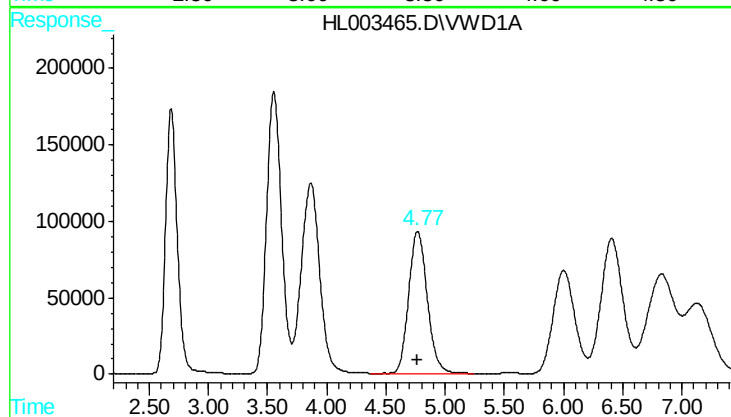


#12 Nitrobenzene

R.T.: 4.768 min
Delta R.T.: 0.000 min
Response: 10267637
Conc: 998.66 ug/L

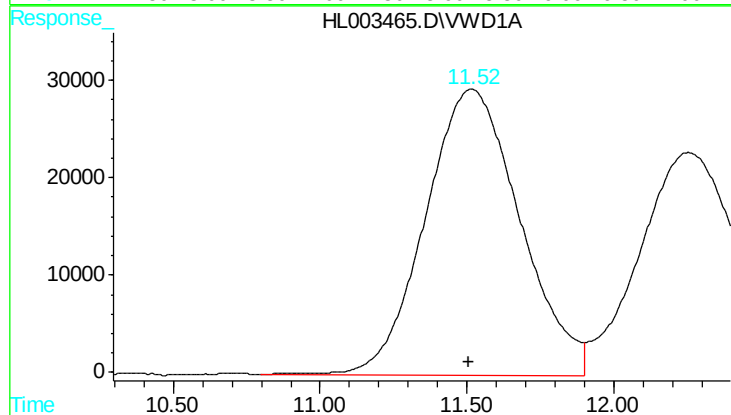

#13 2-Nitrotoluene


R.T.: 11.516 min
Delta R.T.: 0.009 min
Response: 6586871
Conc: 998.82 ug/L

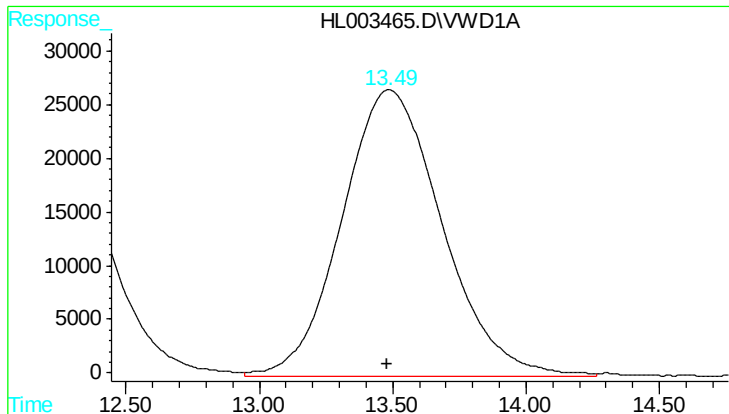

#14 3-Nitrotoluene


R.T.: 13.489 min
Delta R.T.: 0.007 min
Response: 6999051
Conc: 989.65 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL091912

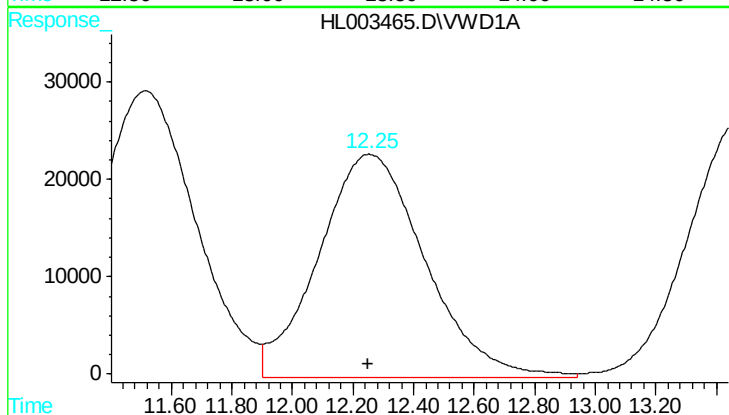


#15 4-Nitrotoluene

R.T.: 12.254 min
Delta R.T.: 0.005 min
Response: 5594790
Conc: 1013.58 ug/L

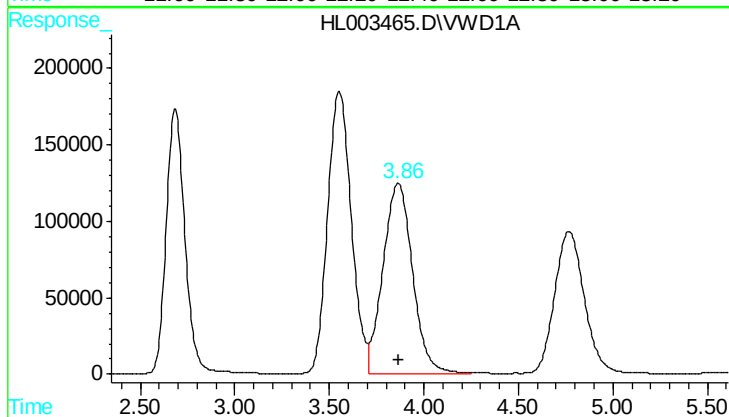


#16 3,5-Dinitroaniline

R.T.: 3.866 min
Delta R.T.: -0.001 min
Response: 13551587
Conc: 886.07 ug/L

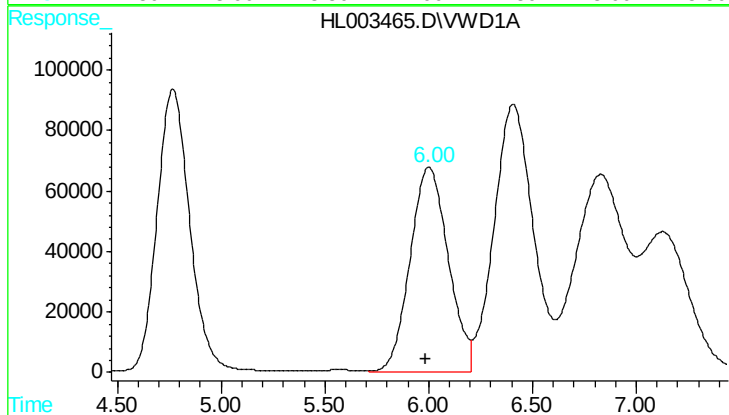

#17 Nitroglycerin

R.T.: 6.002 min
Delta R.T.: 0.015 min
Response: 8668448
Conc: 152638.96 ug/L

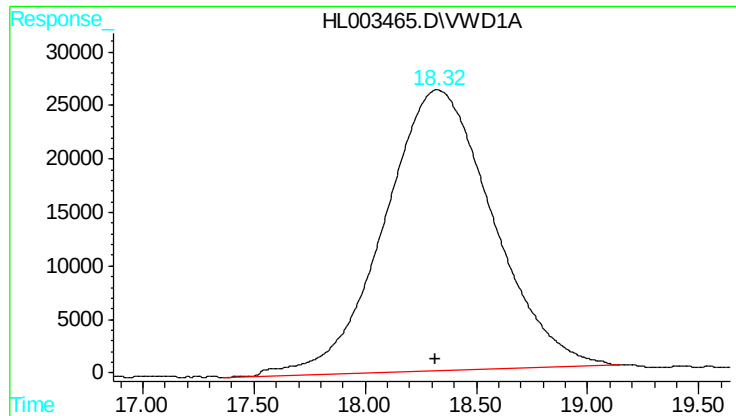

#18 PETN

R.T.: 18.324 min
Delta R.T.: 0.011 min
Response: 8958669
Conc: 925.95 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL091912