

Data File : H:\VOL1\HPLC\HPLC L\120919\HL003485.D Vial: 11
Acq On : 20-Sep-2012, 00:38 Operator: HLM
Sample : 8330NG-CCV Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Sep 20 8:36 2012 Quant Results File: HL091912.RES

Instrument :
HPLC_L
LabSampleId :
8330NG-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Thu Sep 20 08:25:48 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

5) T	Tetryl	6.01	562429	65.897 ug/L
17) T	Nitroglycerin	6.01	562429	9903.562 ug/L


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\120919\HL003485.D Vial: 11
 Acq On : 20-Sep-2012, 00:38 Operator: HLM
 Sample : 8330NG-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Sep 20 8:36 2012 Quant Results File: HL091912.RES

Instrument :
 HPLC_L
 LabSampleId :
 8330NG-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Thu Sep 20 08:25:48 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

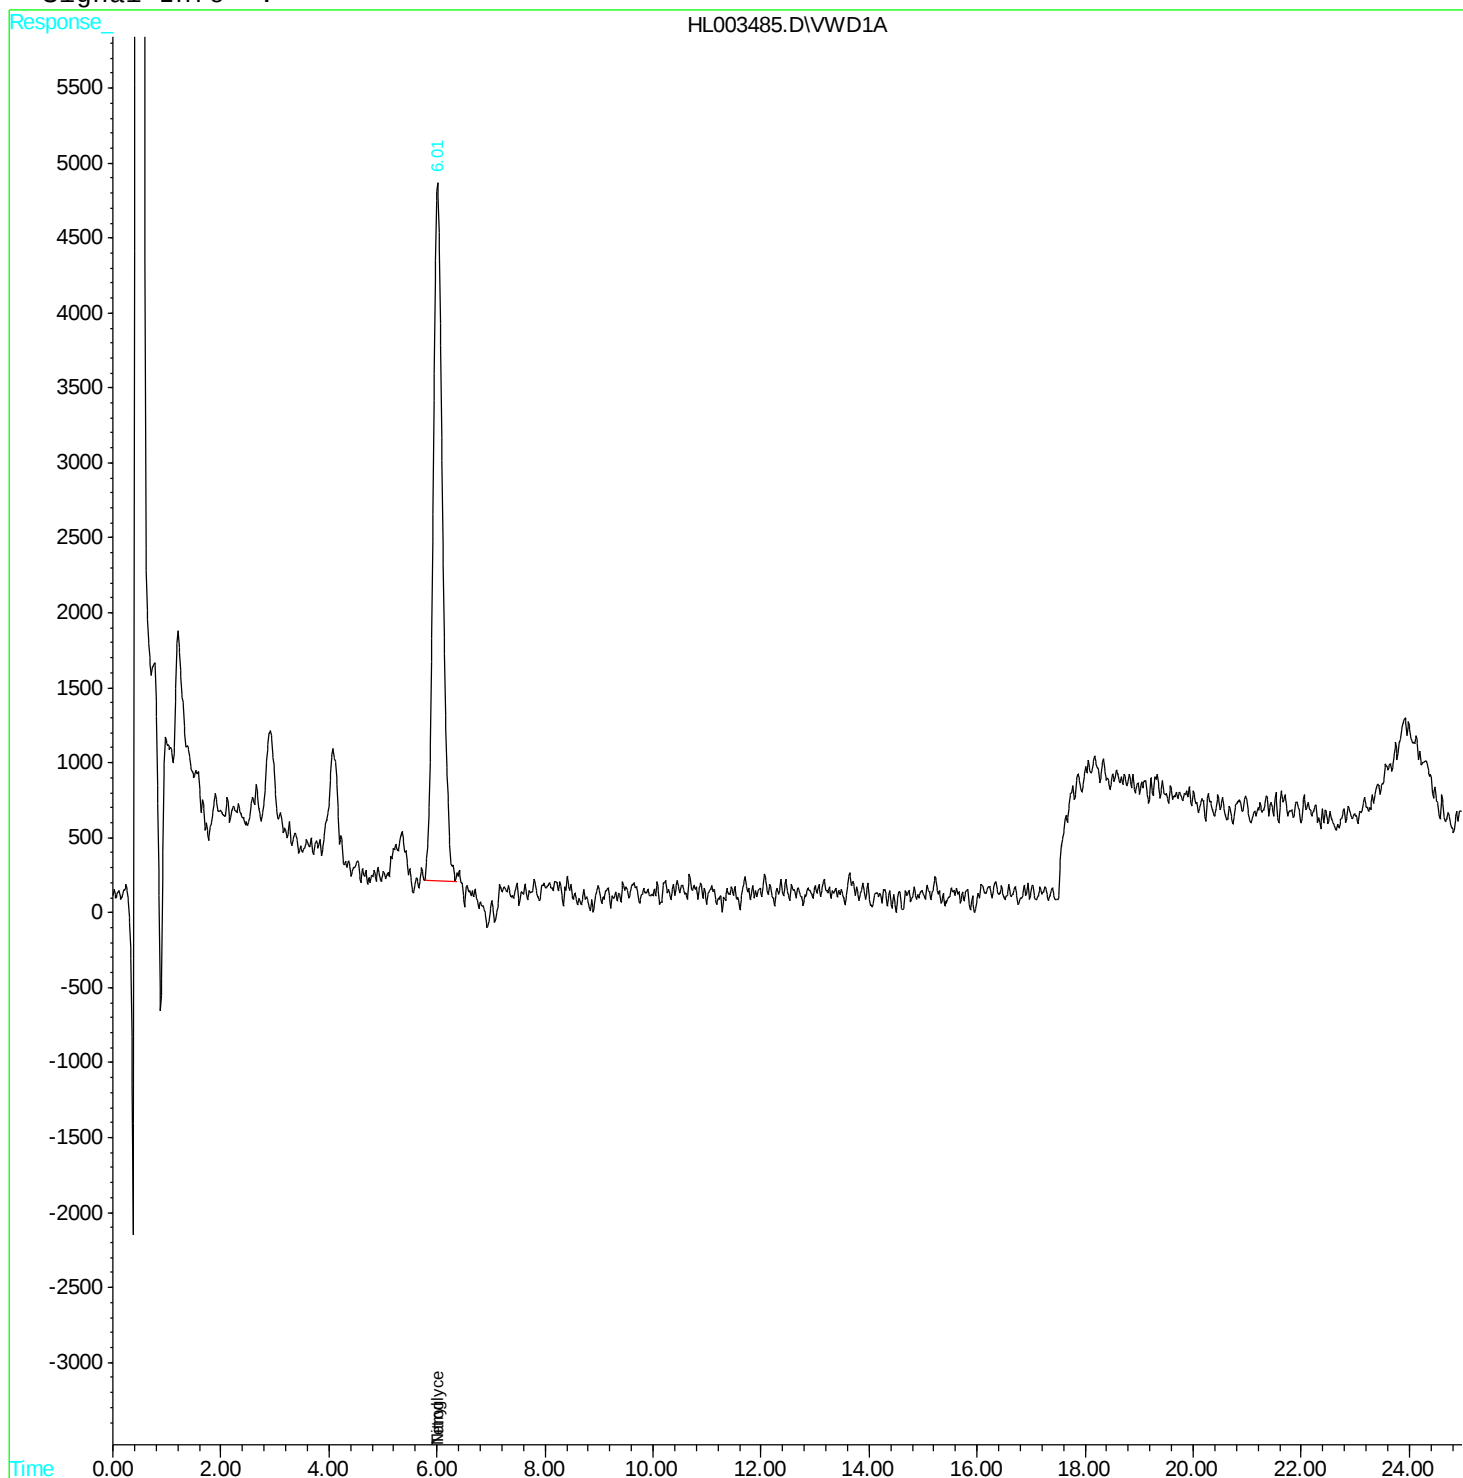


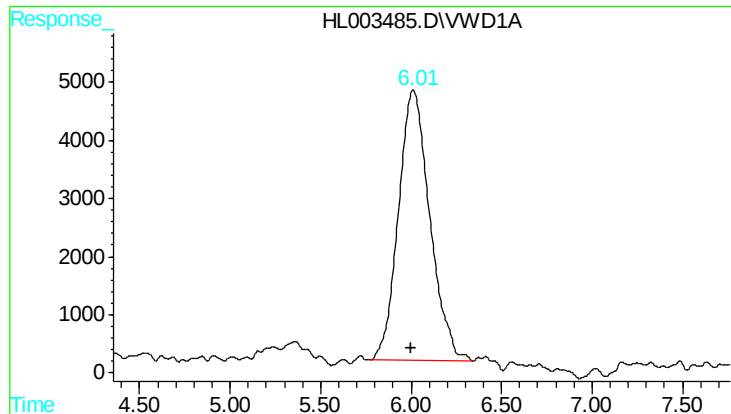

#5 Tetryl

R.T.: 6.012 min
Delta R.T.: 0.014 min
Response: 562429
Conc: 65.90 ug/L

Instrument :
HPLC_L
LabSampleId :
8330NG-CCV

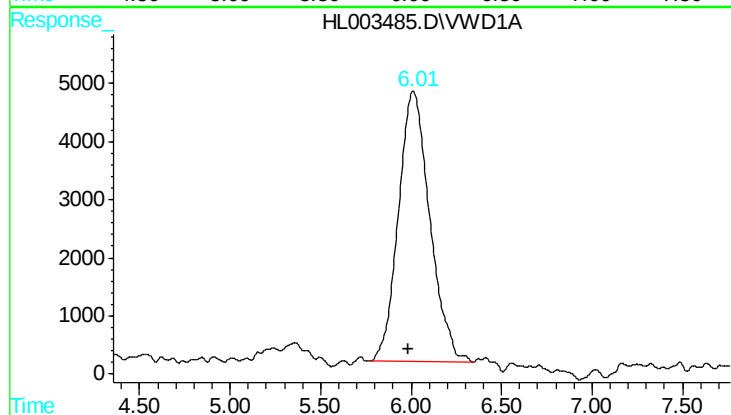

#17 Nitroglycerin

R.T.: 6.012 min
Delta R.T.: 0.026 min
Response: 562429
Conc: 9903.56 ug/L