

Data Path : X:\HPCHEM1\HPLC_L\Data\HL091912\
 Data File : HL003465.D
 Signal(s) : VWD1A.CH
 Acq On : 19-Sep-2012, 15:40
 Operator : HLM
 Sample : 8330-ICV
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 ICVHL091912

Integration File: events.e
 Quant Time: Sep 24 07:56:13 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Thu Sep 20 08:25:48 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc	Units

System Monitoring Compounds				
Target Compounds				
2) T HMX	0.899	3986103	1018.959	ug/L
3) T RDX	1.723	5422894	1042.827	ug/L
4) T 1,3,5-Trinitrobenzene	2.685	11955725	984.794	ug/L
5) T Tetryl	6.002	8668448	1015.642	ug/L
6) T 2,4,6-Trinitrotoluene	6.408	11559836	1025.901	ug/L
7) T 2-Amino-4,6-dinitroto...	6.829	10793070	991.503	ug/L
8) T 4-Amino-2,6-dinitroto...	7.128	7387679	1069.044	ug/L
9) T 2,4-Dinitrotoluene	7.992	14496101	960.368	ug/L
10) T 2,6-Dinitrotoluene	8.348	8297636	953.293	ug/L
11) T 1,3-Dinitrobenzene	3.553	16037768	1012.316	ug/L
12) T Nitrobenzene	4.768	10267637	998.660	ug/L
13) T 2-Nitrotoluene	11.516	6586871	998.823	ug/L
14) T 3-Nitrotoluene	13.489	6999051	989.654	ug/L
15) T 4-Nitrotoluene	12.254	5594790	1013.579	ug/L
16) T 3,5-Dinitroaniline	3.866	13551587	886.073	ug/L
18) T PETN	18.324	8958669	925.954	ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : X:\HPCHEM1\HPLC_L\Data\HL091912\
Data File : HL003465.D
Signal(s) : VWD1A.CH
Acq On : 19-Sep-2012, 15:40
Operator : HLM
Sample : 8330-ICV
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
ICVHL091912

Integration File: events.e
Quant Time: Sep 24 07:56:13 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Sep 20 08:25:48 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

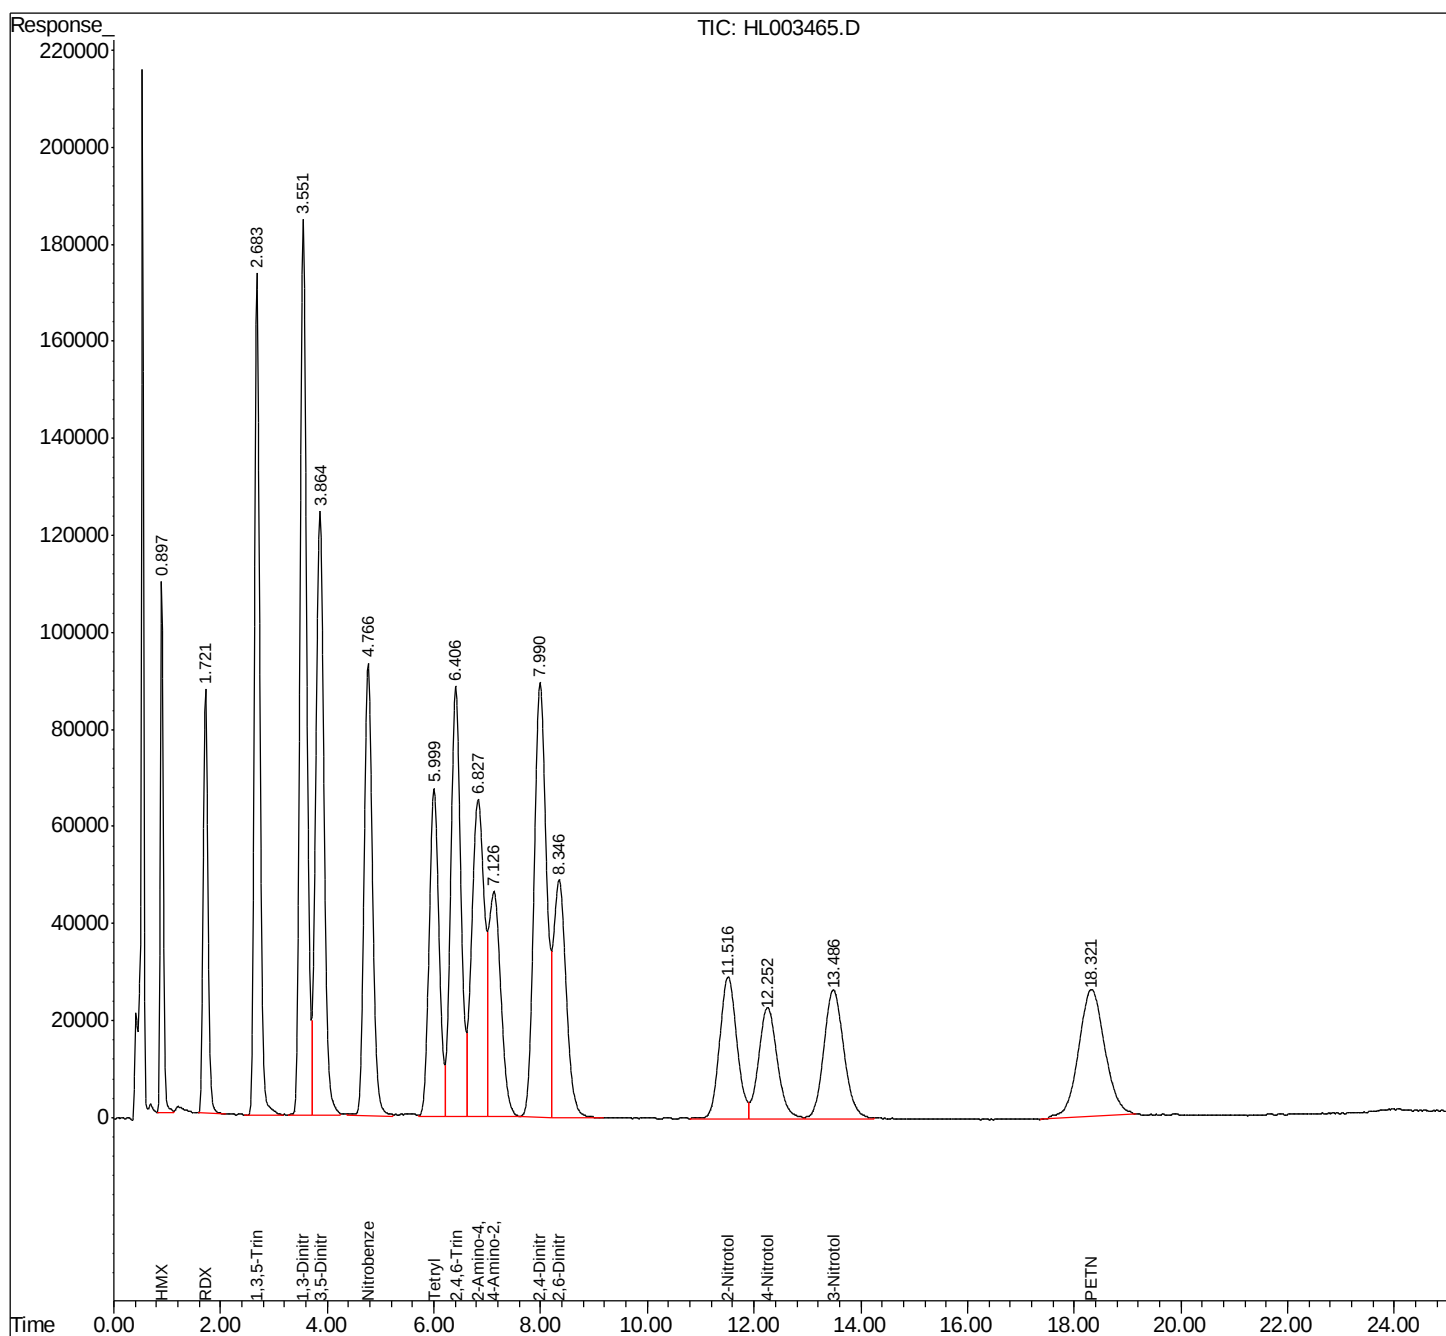


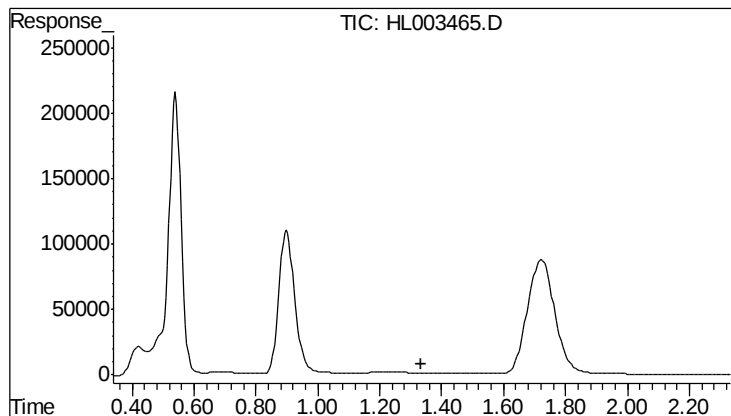

#1 4-Nitroaniline


R.T.: 0.000 min
 Exp R.T.: 1.335 min
 Response: 0
 Conc: N.D.

Instrument :
 HPLC_L
 ClientSampleId :
 ICVHL091912

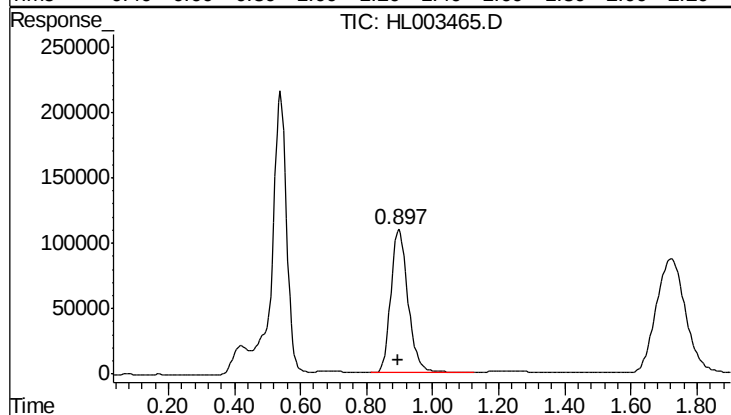


#2 HMX

R.T.: 0.899 min
 Delta R.T.: 0.003 min
 Response: 3986103
 Conc: 1018.96 ug/L

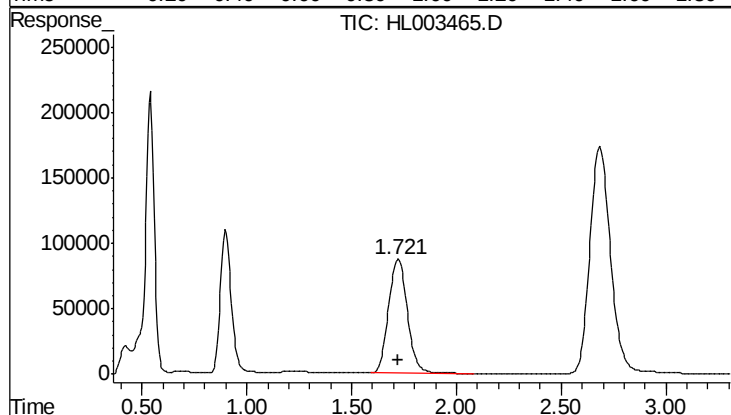


#3 RDX

R.T.: 1.723 min
 Delta R.T.: 0.003 min
 Response: 5422894
 Conc: 1042.83 ug/L

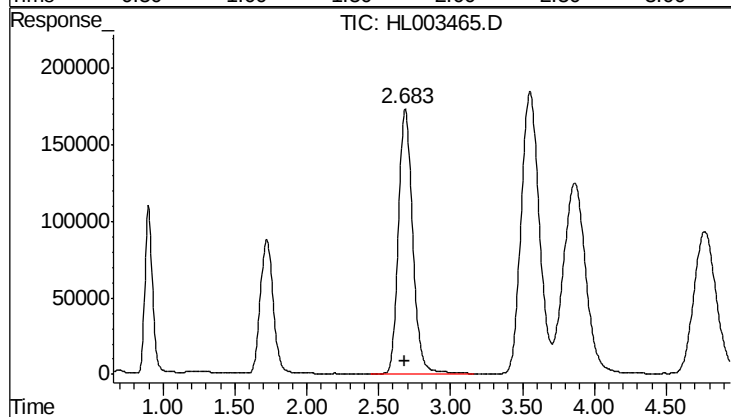

#4 1,3,5-Trinitrobenzene


R.T.: 2.685 min
 Delta R.T.: 0.002 min
 Response: 11955725
 Conc: 984.79 ug/L

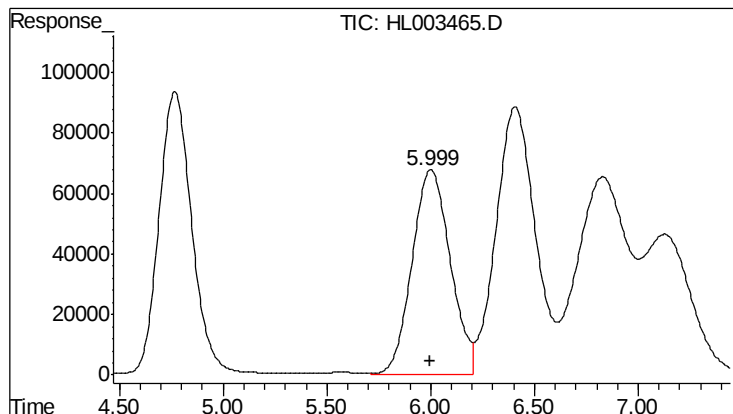

#5 Tetryl


R.T.: 6.002 min
Delta R.T.: 0.003 min
Response: 8668448
Conc: 1015.64 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL091912

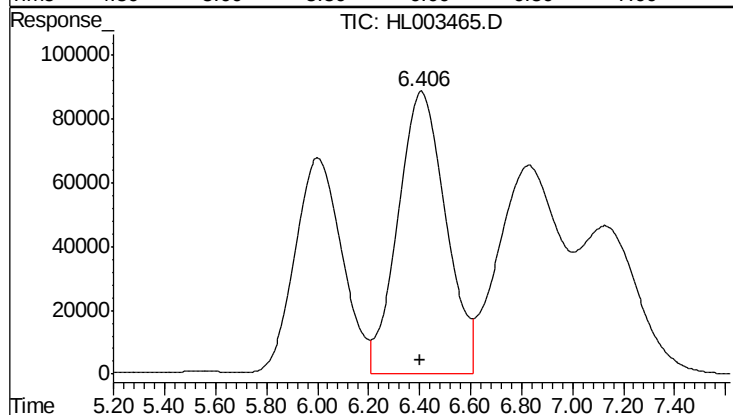


#6 2,4,6-Trinitrotoluene

R.T.: 6.408 min
Delta R.T.: 0.004 min
Response: 11559836
Conc: 1025.90 ug/L

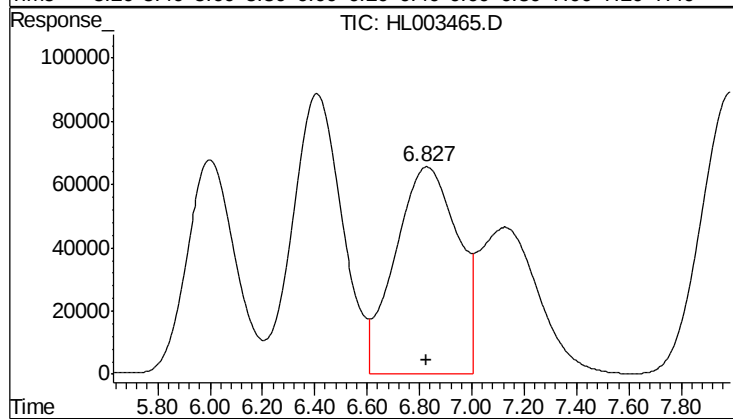


#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.829 min
Delta R.T.: 0.003 min
Response: 10793070
Conc: 991.50 ug/L

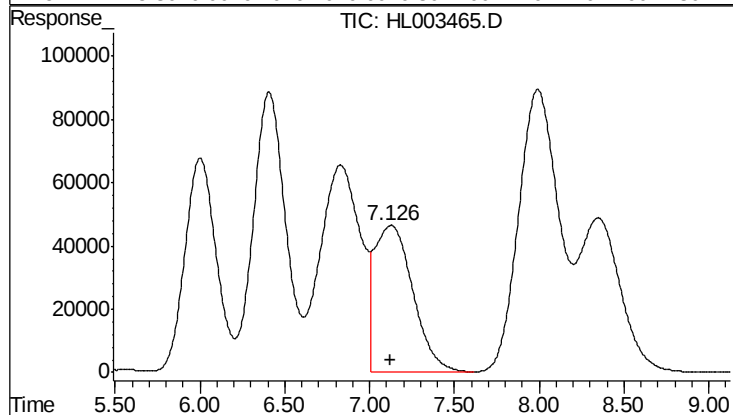

#8 4-Amino-2,6-dinitrotoluene


R.T.: 7.128 min
Delta R.T.: 0.002 min
Response: 7387679
Conc: 1069.04 ug/L

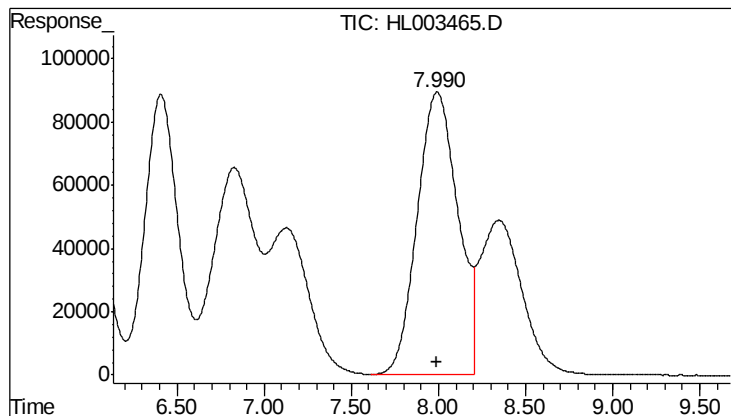

#9 2,4-Dinitrotoluene


R.T.: 7.992 min
Delta R.T.: 0.004 min
Response: 14496101
Conc: 960.37 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL091912

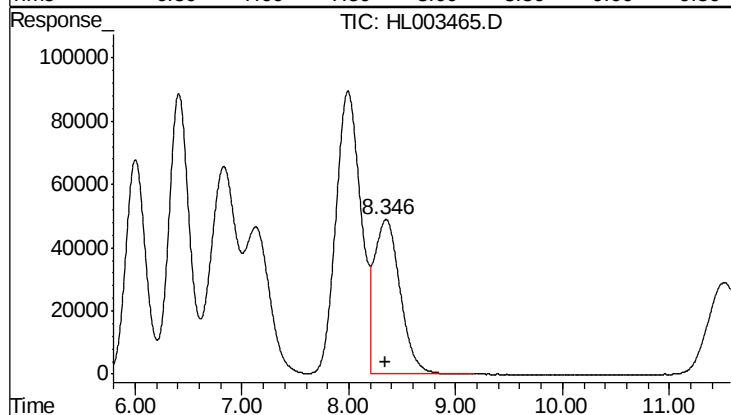


#10 2,6-Dinitrotoluene

R.T.: 8.348 min
Delta R.T.: 0.005 min
Response: 8297636
Conc: 953.29 ug/L

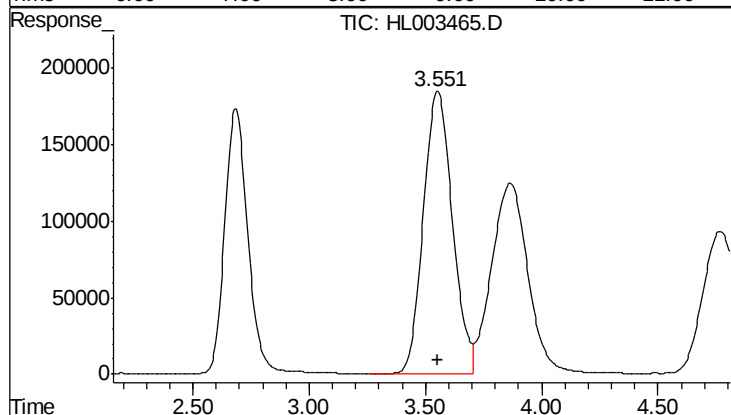


#11 1,3-Dinitrobenzene

R.T.: 3.553 min
Delta R.T.: 0.000 min
Response: 16037768
Conc: 1012.32 ug/L

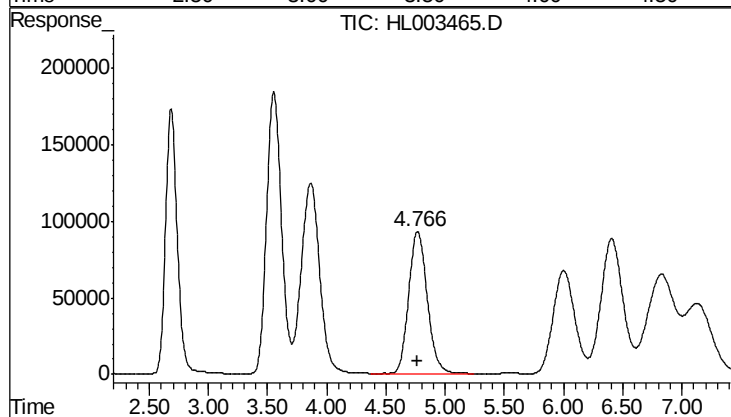

#12 Nitrobenzene


R.T.: 4.768 min
Delta R.T.: 0.000 min
Response: 10267637
Conc: 998.66 ug/L

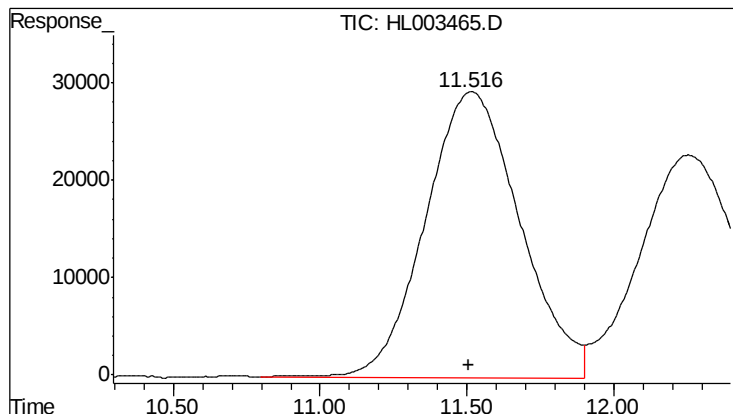

#13 2-Nitrotoluene


R.T.: 11.516 min
 Delta R.T.: 0.009 min
 Response: 6586871
 Conc: 998.82 ug/L

Instrument :
 HPLC_L
 ClientSampleId :
 ICVHL091912

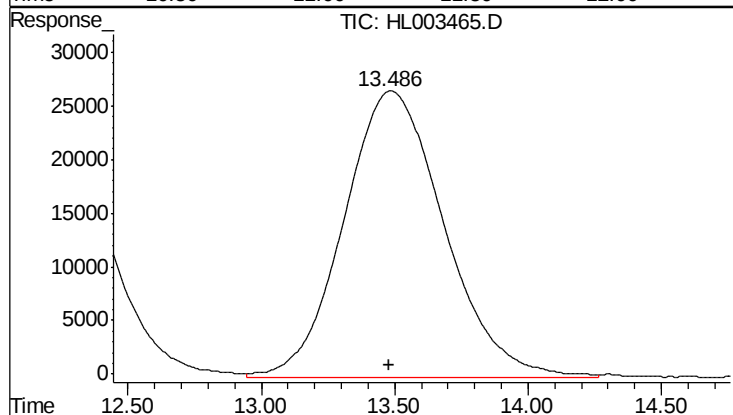


#14 3-Nitrotoluene

R.T.: 13.489 min
 Delta R.T.: 0.007 min
 Response: 6999051
 Conc: 989.65 ug/L

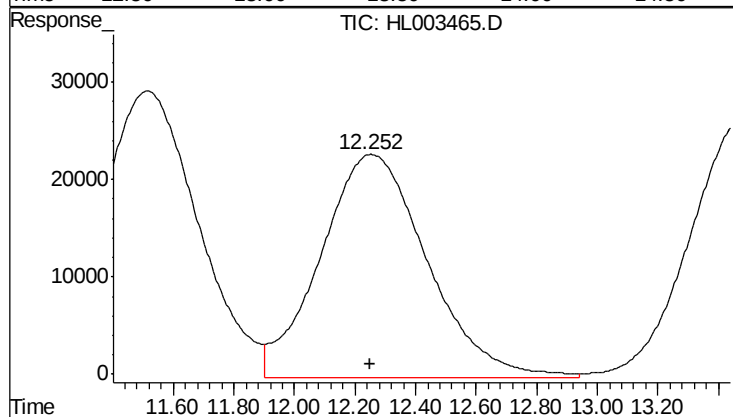


#15 4-Nitrotoluene

R.T.: 12.254 min
 Delta R.T.: 0.005 min
 Response: 5594790
 Conc: 1013.58 ug/L

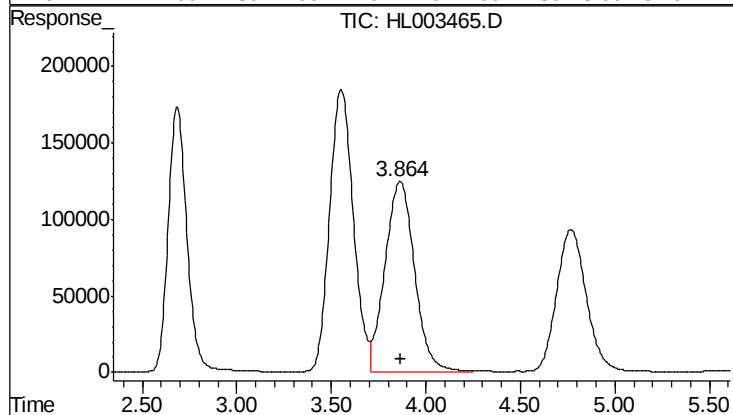

#16 3,5-Dinitroaniline

R.T.: 3.866 min
 Delta R.T.: -0.001 min
 Response: 13551587
 Conc: 886.07 ug/L

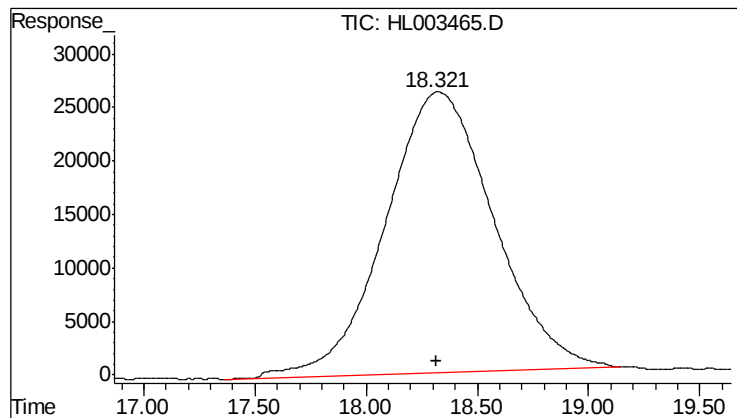

#18 PETN

R.T.: 18.324 min
Delta R.T.: 0.011 min
Response: 8958669
Conc: 925.95 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL091912