

Data Path : X:\HPCHEM1\HPLC_L\Data\HL091912\
Data File : HL003490.D
Signal(s) : VWD1A.CH
Acq On : 20-Sep-2012, 02:53
Operator : HLM
Sample : D4129-02
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HELIPORTCOMP2

Manual Integrations
APPROVED

AHPatel
9/25/2012 4:13:00 AM

Integration File: events.e
Quant Time: Sep 24 07:58:25 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Sep 20 08:25:48 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.334	622774	167.615 ug/L m
Spiked Amount 300.000	Range 37 - 149	Recovery =	55.87%
Target Compounds			

(f)=RT Delta > 1/2 Window		(m)=manual int.	

Data Path : X:\HPCHEM1\HPLC_L\Data\HL091912\
Data File : HL003490.D
Signal(s) : VWD1A.CH
Acq On : 20-Sep-2012, 02:53
Operator : HLM
Sample : D4129-02
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
HELIORTCOMP2


Manual Integrations
APPROVED

AHPatel
9/25/2012 4:13:00 AM

Integration File: events.e
Quant Time: Sep 24 07:58:25 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Sep 20 08:25:48 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

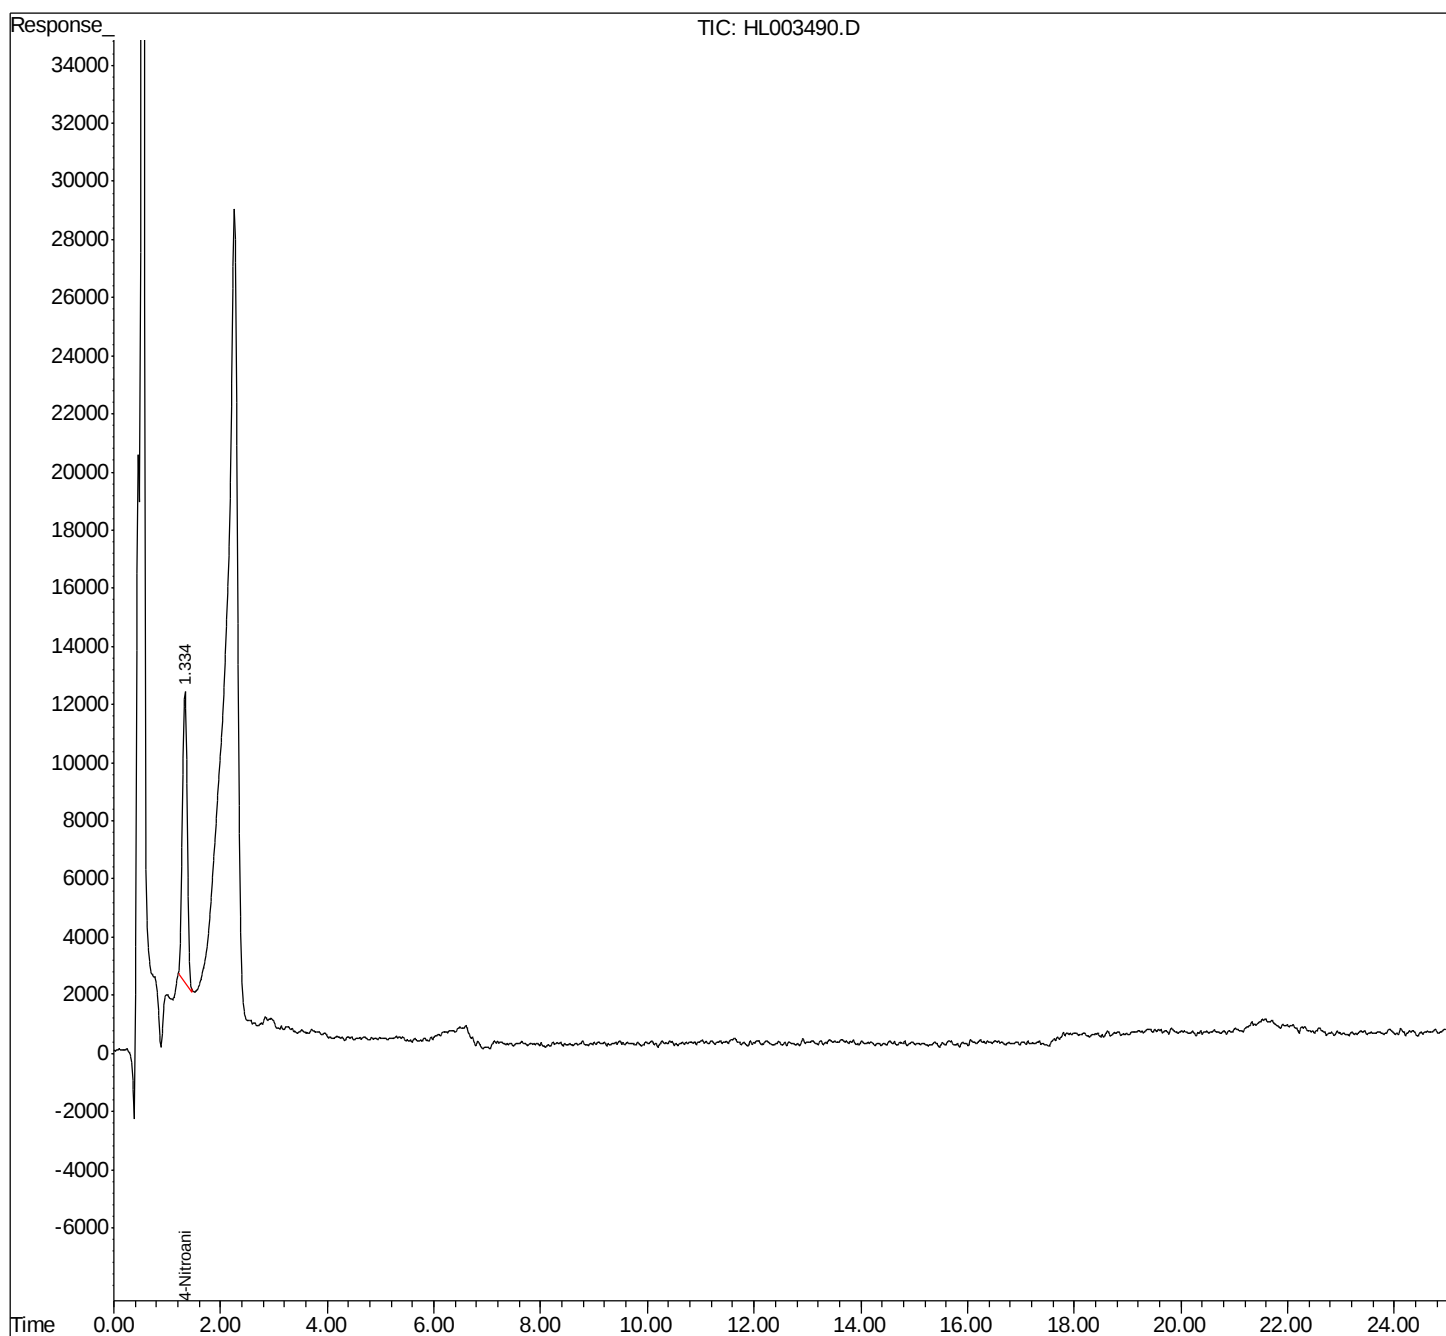

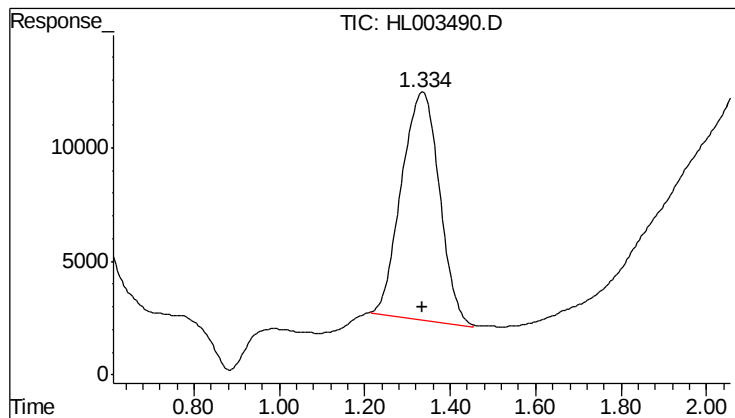

#1 4-Nitroaniline

R.T.: 1.334 min
Delta R.T.: 0.000 min
Response: 622774
Conc: 167.61 ug/L m

Instrument :
HPLC_L
ClientSampleId :
HELIPORTCOMP2

Manual Integrations
APPROVED

AHPatel
9/25/2012 4:13:00 AM