

Data Path : X:\HPCHEM1\HPLC_L\Data\HL091912\
Data File : HL003492.D
Signal(s) : VWD1A.CH
Acq On : 20-Sep-2012, 03:47
Operator : HLM
Sample : D4129-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HELIPORTCOMP4

Manual Integrations
APPROVED

AHPatel
9/25/2012 4:13:06 AM

Integration File: events.e
Quant Time: Sep 24 07:58:38 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Sep 20 08:25:48 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.331	869165	233.929 ug/L m
Spiked Amount 300.000	Range 37 - 149	Recovery =	77.98%
Target Compounds			

(f)=RT Delta > 1/2 Window (m)=manual int.

Data Path : X:\HPCHEM1\HPLC_L\Data\HL091912\
Data File : HL003492.D
Signal(s) : VWD1A.CH
Acq On : 20-Sep-2012, 03:47
Operator : HLM
Sample : D4129-04
Misc :
ALS Vial : 37 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
HELIPORTCOMP4


Manual Integrations
APPROVED

AHPatel
9/25/2012 4:13:06 AM

Integration File: events.e
Quant Time: Sep 24 07:58:38 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Sep 20 08:25:48 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

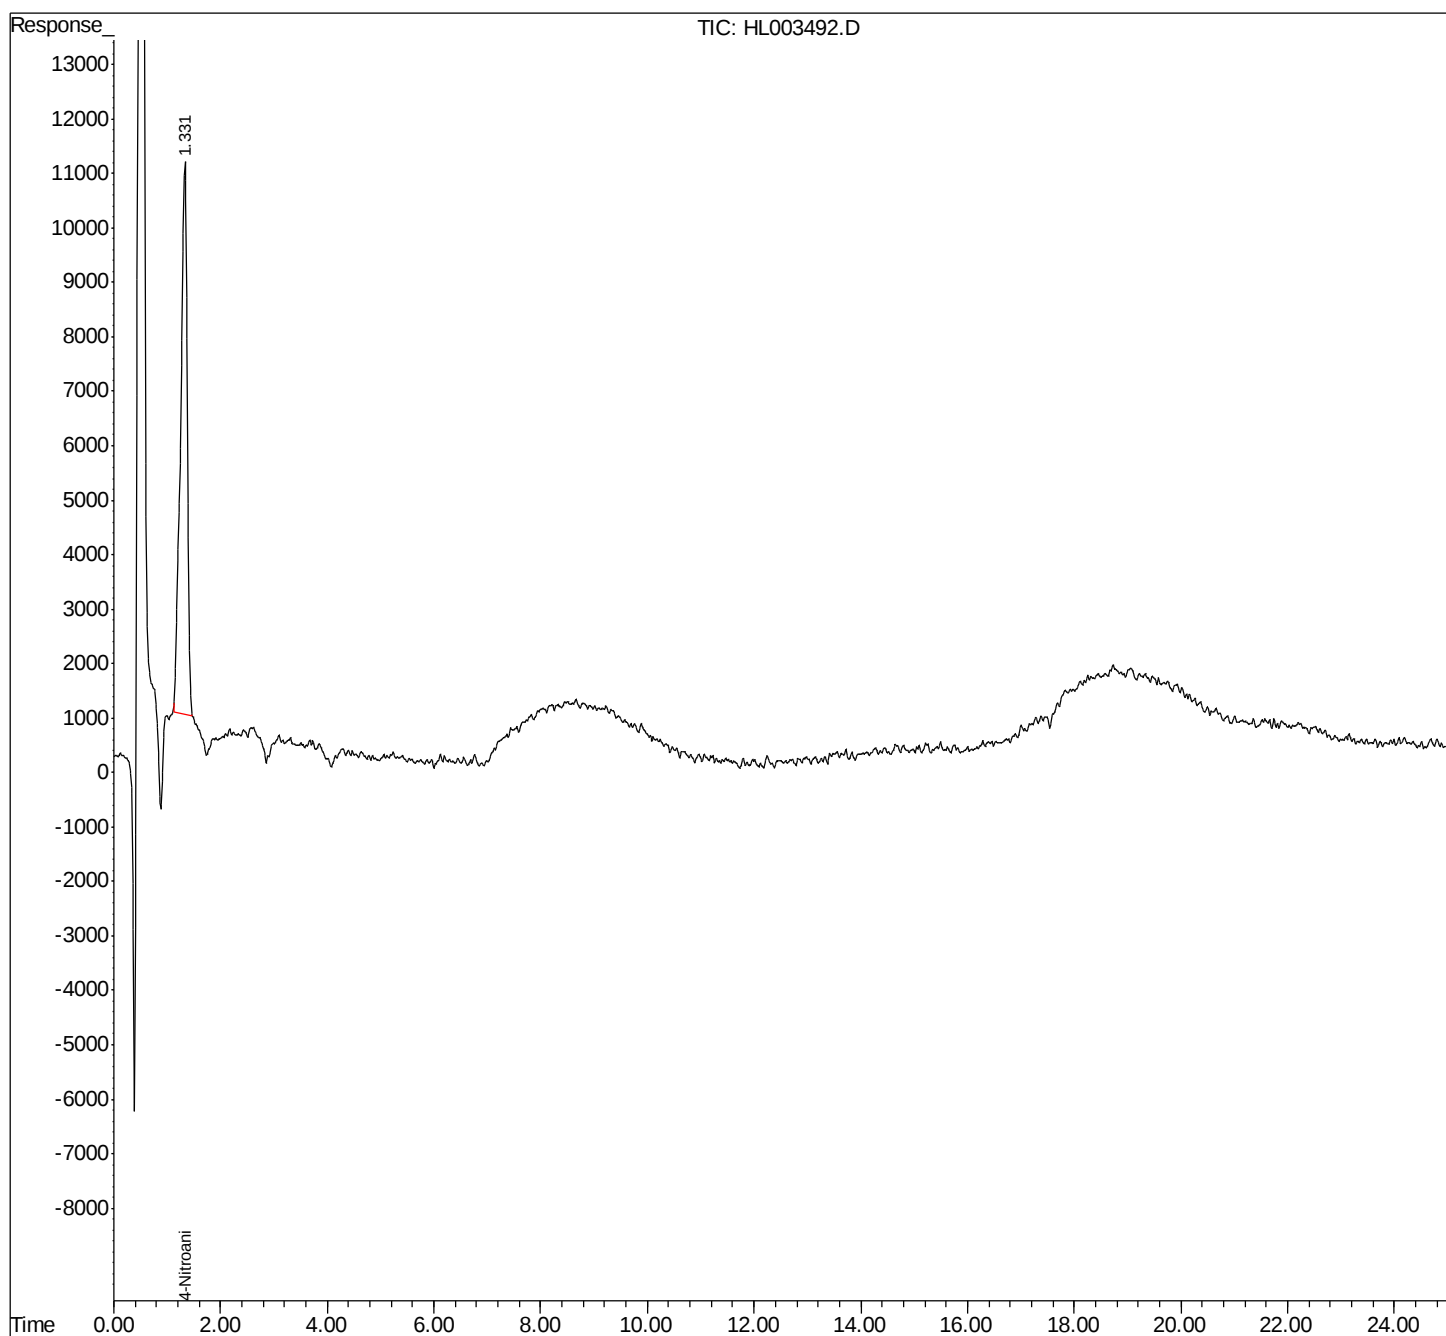

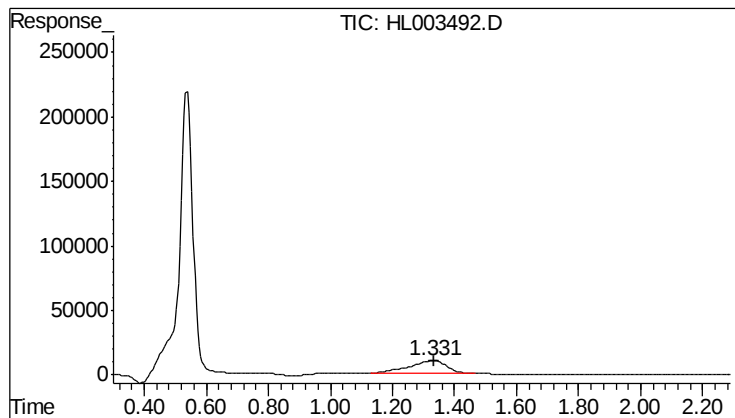

#1 4-Nitroaniline

R.T.: 1.331 min
Delta R.T.: -0.003 min
Response: 869165
Conc: 233.93 ug/L m

Instrument :
HPLC_L
ClientSampleId :
HELIPORTCOMP4

Manual Integrations
APPROVED

AHPatel
9/25/2012 4:13:06 AM