

Data File : H:\VOL1\HPLC\HPLC L\120920\HL003510.D Vial: 47
 Acq On : 20-Sep-2012, 12:32 Operator: HLM
 Sample : PB65762BS2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Sep 21 13:04 2012 Quant Results File: HL091912.RES

Instrument :
 HPLC_L
 ClientSampleId :
 PB65762BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Fri Sep 21 13:01:00 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	554865	149.338 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 49.78%

Target Compounds

5) T	Tetryl	6.10	134052	15.706 ug/L
17) T	Nitroglycerin	6.10	134052	2360.469 ug/L
18) T	PETN	18.57f	3033	0.313 ug/L

Data File : H:\VOL1\HPLC\HPLC L\120920\HL003510.D

Vial: 47

Acq On : 20-Sep-2012, 12:32

Operator: HLM

Sample : PB65762BS2

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Sep 21 13:04 2012 Quant Results File: HL091912.RES

Instrument :

HPLC_L

ClientSampleId :

PB65762BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Fri Sep 21 13:01:00 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

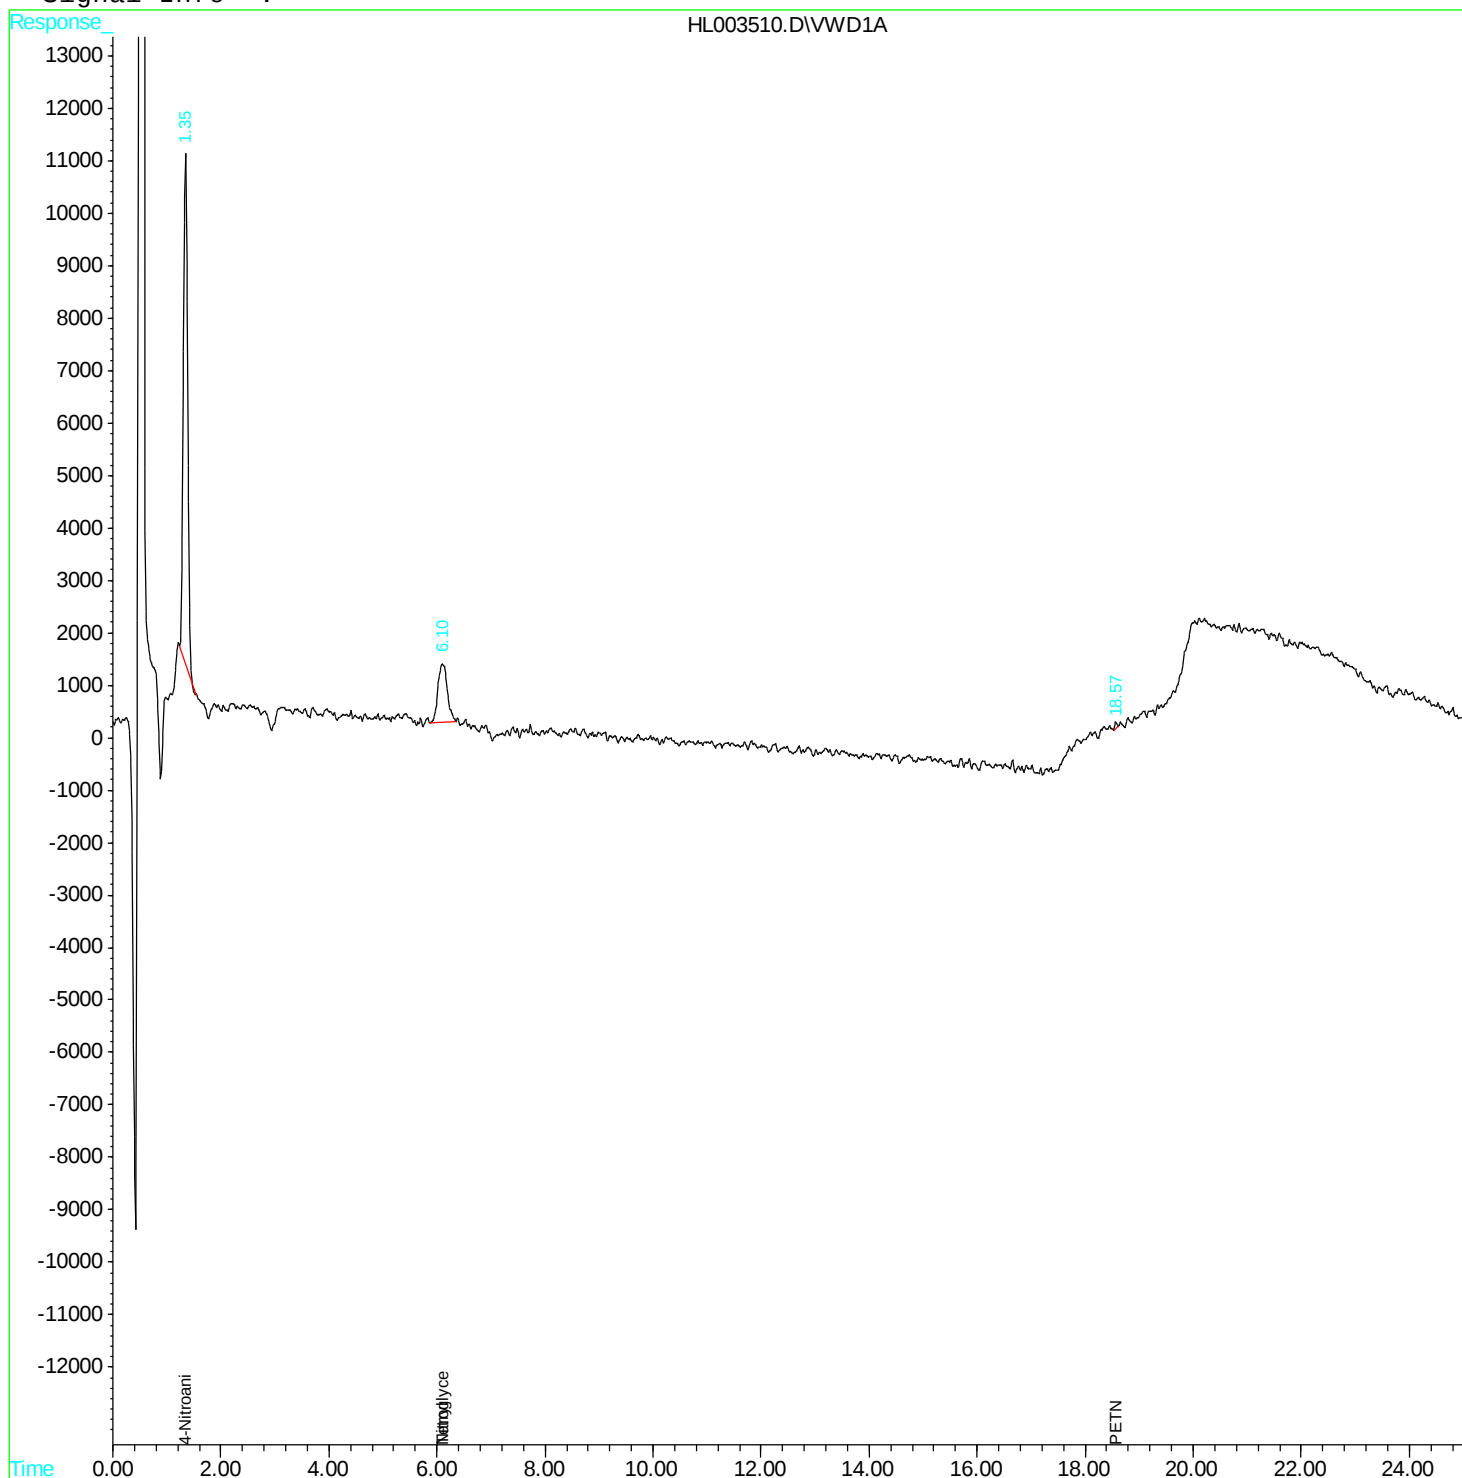


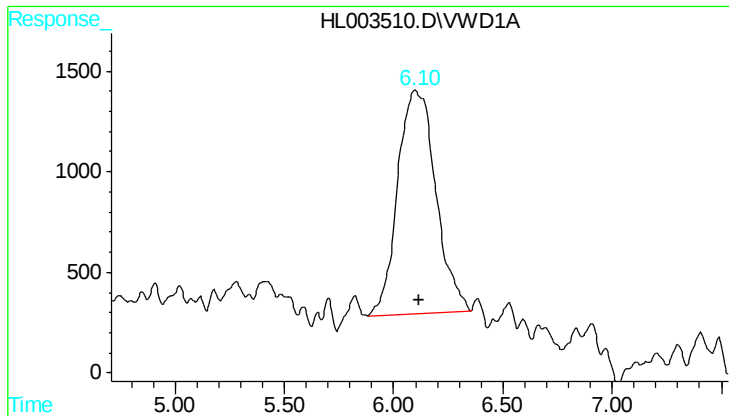

#5 Tetryl


R.T.: 6.099 min
Delta R.T.: -0.018 min
Response: 134052
Conc: 15.71 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB65762BS2

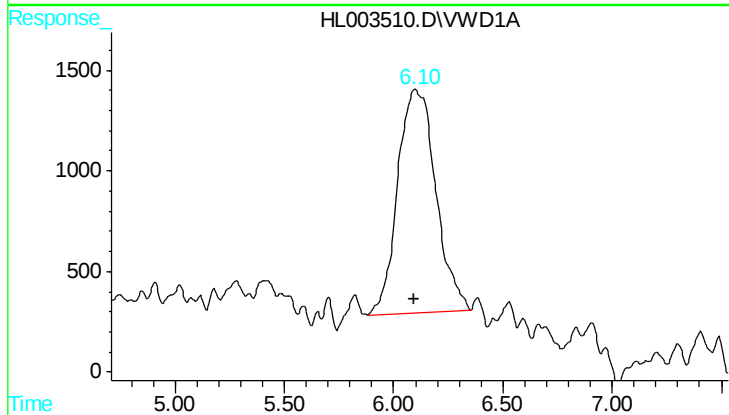

#17 Nitroglycerin

R.T.: 6.099 min
Delta R.T.: 0.003 min
Response: 134052
Conc: 2360.47 ug/L

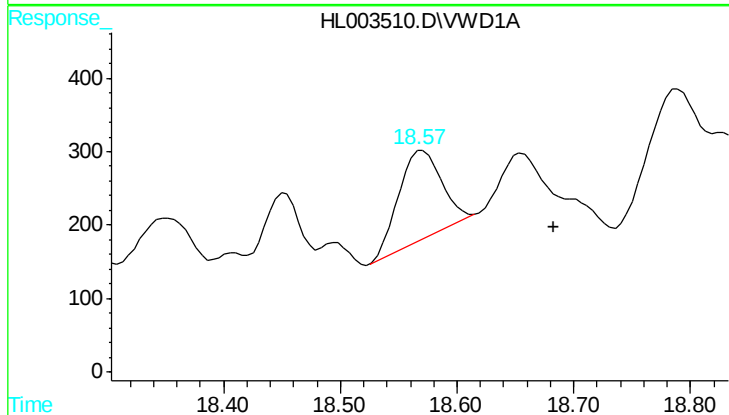

#18 PETN

R.T.: 18.571 min
Delta R.T.: -0.111 min
Response: 3033
Conc: 0.31 ug/L