

Data File : H:\VOL1\HPLC\HPLC L\120920\HL003523.D Vial: 57
Acq On : 20-Sep-2012, 18:22 Operator: HLM
Sample : PB65783BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Sep 21 13:05 2012 Quant Results File: HL091912.RES

Instrument :
HPLC_L
ClientSampleId :
PB65783BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Fri Sep 21 13:01:00 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	1259845	339.077 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 113.03%

Target Compounds


5) T	Tetryl	6.10	292705	34.295 ug/L
17) T	Nitroglycerin	6.10	292705	5154.120 ug/L


Data File : H:\VOL1\HPLC\HPLC L\120920\HL003523.D Vial: 57
Acq On : 20-Sep-2012, 18:22 Operator: HLM
Sample : PB65783BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Sep 21 13:05 2012 Quant Results File: HL091912.RES

Instrument :
HPLC_L
ClientSampleId :
PB65783BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Fri Sep 21 13:01:00 2012
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

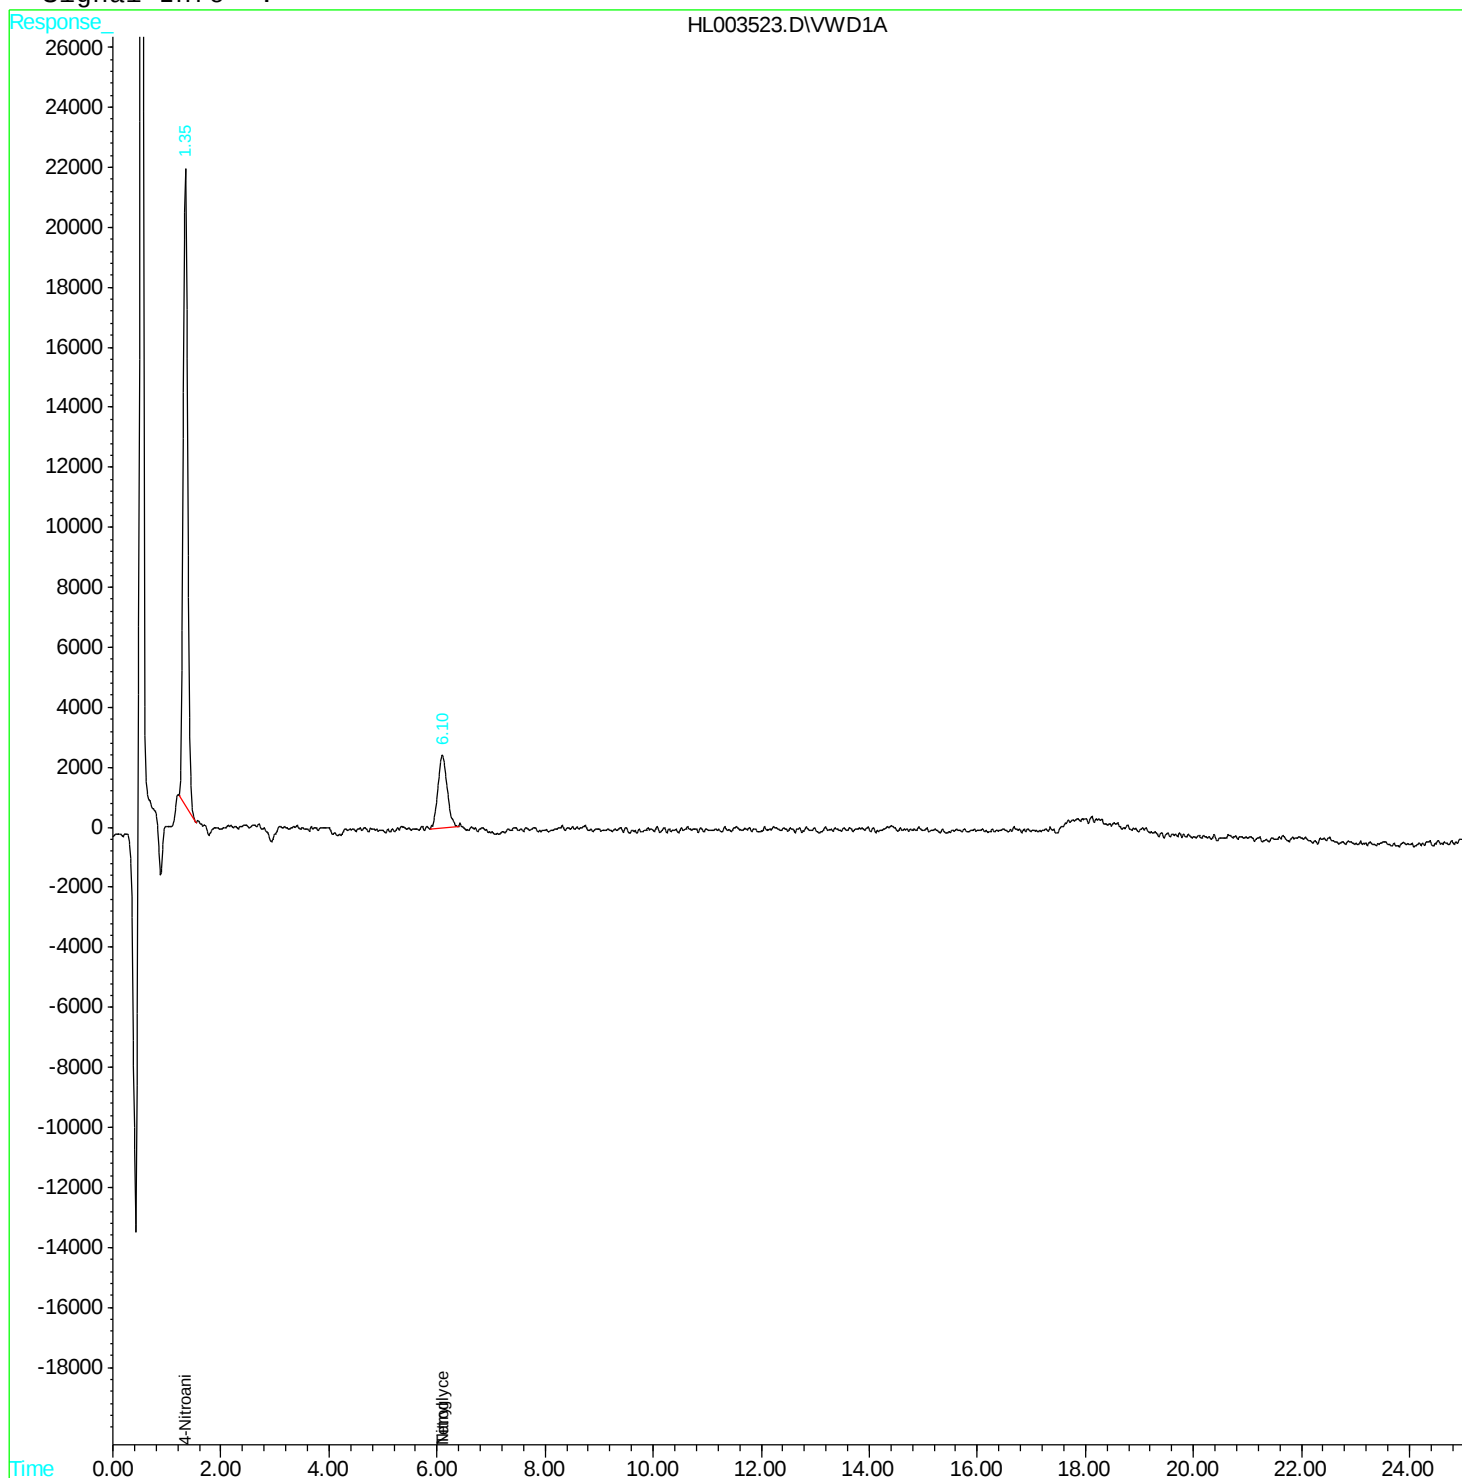


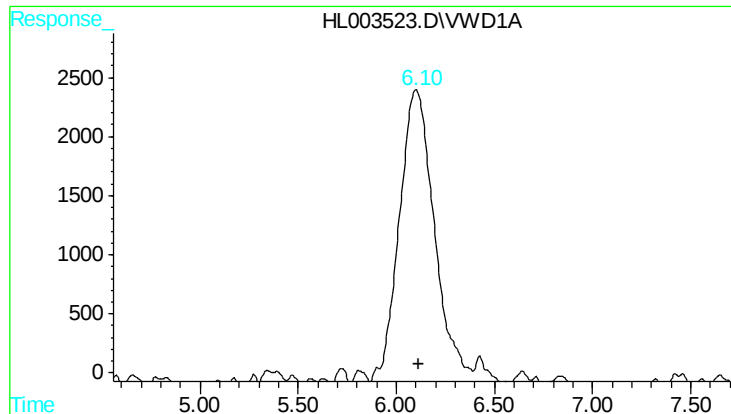

#5 Tetryl

R.T.: 6.100 min
Delta R.T.: -0.017 min
Response: 292705
Conc: 34.29 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB65783BS2

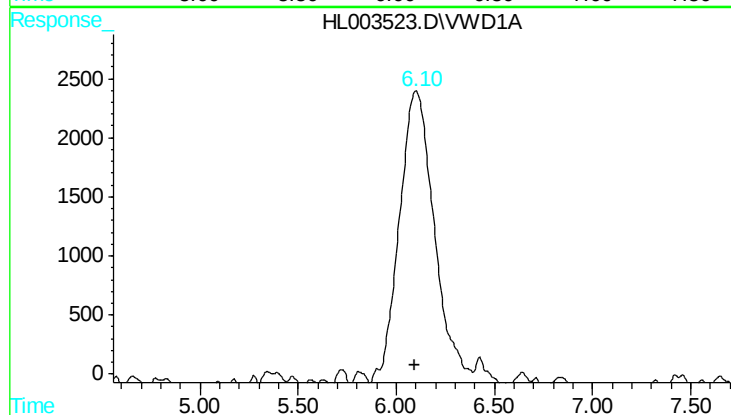

#17 Nitroglycerin

R.T.: 6.100 min
Delta R.T.: 0.005 min
Response: 292705
Conc: 5154.12 ug/L