

Data File : H:\VOL1\HPLC\HPLC L\120920\HL003525.D Vial: 59  
Acq On : 20-Sep-2012, 19:16 Operator: HLM  
Sample : PB65783BSD2 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : events.e  
Quant Time: Sep 21 13:06 2012 Quant Results File: HL091912.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
PB65783BSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)  
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
Last Update : Fri Sep 21 13:01:00 2012  
Response via : Initial Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. :  
Signal Phase :  
Signal Info :

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----

System Monitoring Compounds

|               |                |       |          |                    |
|---------------|----------------|-------|----------|--------------------|
| 1) S          | 4-Nitroaniline | 1.35  | 1230739  | 331.244 ug/L       |
| Spiked Amount | 300.000        | Range | 37 - 149 | Recovery = 110.41% |

Target Compounds


|       |               |      |        |               |
|-------|---------------|------|--------|---------------|
| 5) T  | Tetryl        | 6.11 | 290888 | 34.082 ug/L   |
| 17) T | Nitroglycerin | 6.11 | 290888 | 5122.119 ug/L |


Data File : H:\VOL1\HPLC\HPLC L\120920\HL003525.D Vial: 59  
Acq On : 20-Sep-2012, 19:16 Operator: HLM  
Sample : PB65783BSD2 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : events.e  
Quant Time: Sep 21 13:06 2012 Quant Results File: HL091912.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
PB65783BSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)  
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
Last Update : Fri Sep 21 13:01:00 2012  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. :  
Signal Phase :  
Signal Info :

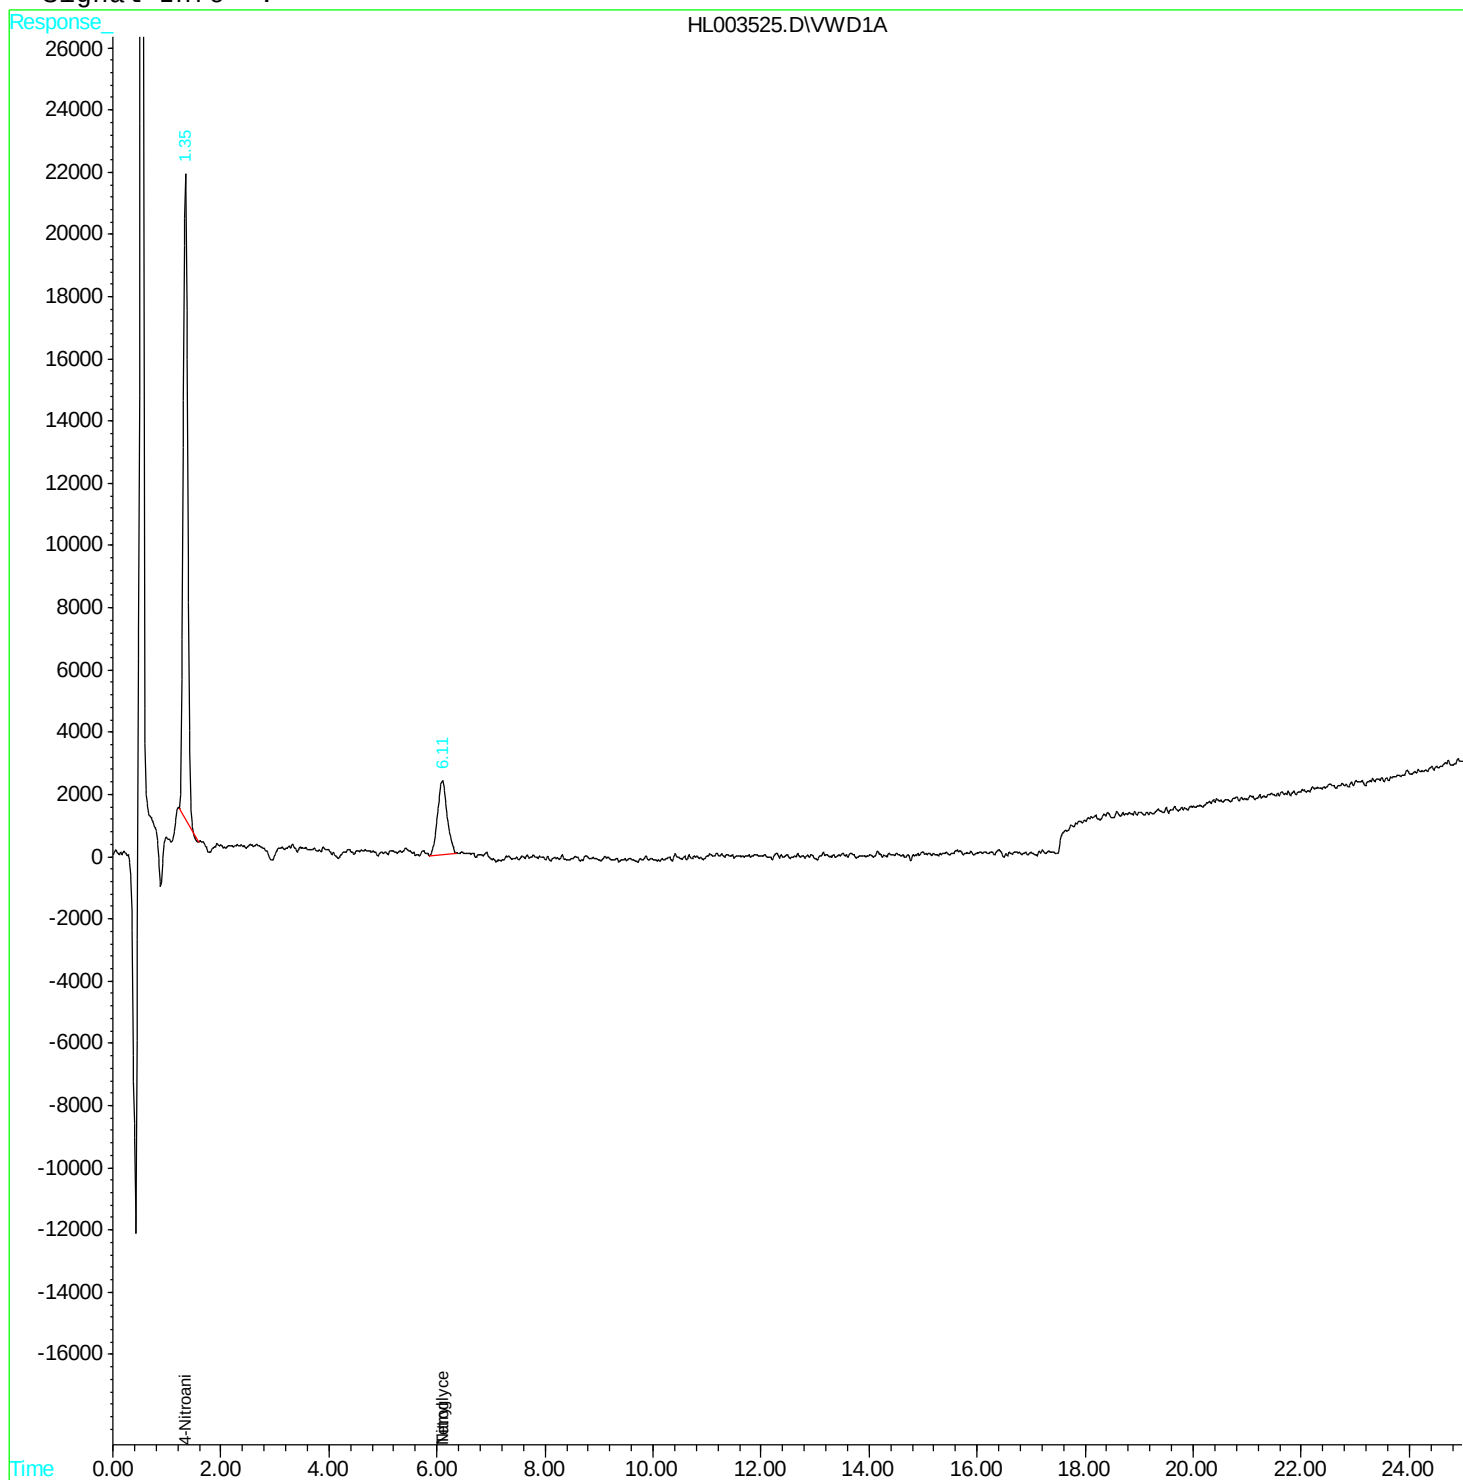


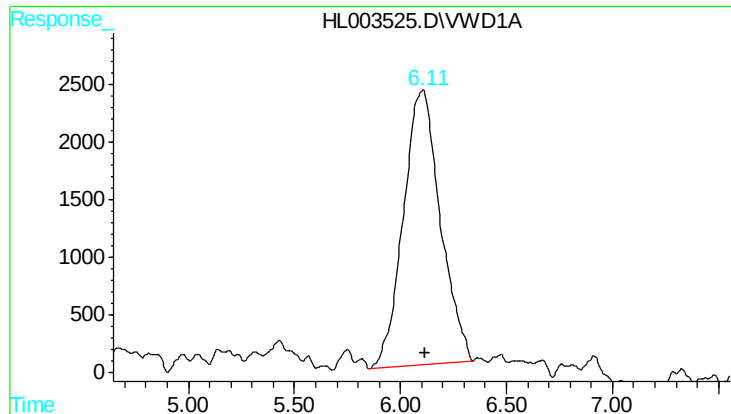

#5 Tetryl

R.T.: 6.107 min  
Delta R.T.: -0.010 min  
Response: 290888  
Conc: 34.08 ug/L

Instrument :  
HPLC\_L  
ClientSampleId :  
PB65783BSD2

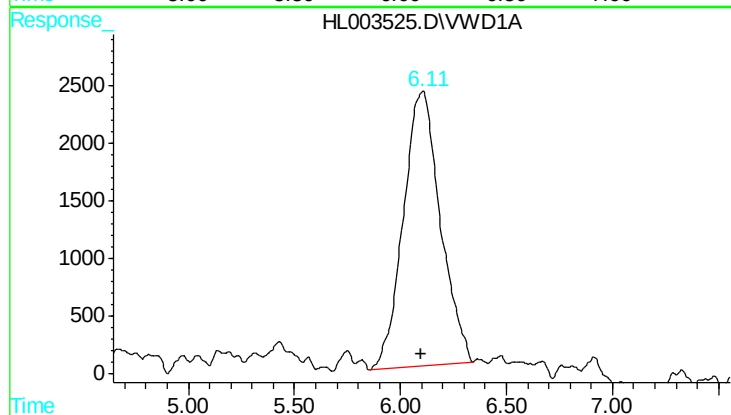

#17 Nitroglycerin

R.T.: 6.107 min  
Delta R.T.: 0.012 min  
Response: 290888  
Conc: 5122.12 ug/L