

Data Path : X:\HPCHEM1\HPLC_L\Data\HL092012\
Data File : HL003507.D
Signal(s) : VWD1A.CH
Acq On : 20-Sep-2012, 11:11
Operator : HLM
Sample : D4131-01
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
BUILDG-B3024COMP2

Manual Integrations
APPROVED

AHPatel
9/25/2012 4:14:14 AM

Integration File: events.e
Quant Time: Sep 24 08:09:25 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Sep 21 13:01:00 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.346	578643	155.737 ug/L m
Spiked Amount 300.000	Range 37 - 149	Recovery =	51.91%
Target Compounds			

(f)=RT Delta > 1/2 Window (m)=manual int.

Data Path : X:\HPCHEM1\HPLC_L\Data\HL092012\
Data File : HL003507.D
Signal(s) : VWD1A.CH
Acq On : 20-Sep-2012, 11:11
Operator : HLM
Sample : D4131-01
Misc :
ALS Vial : 44 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
BUILDG-B3024COMP2


Manual Integrations
APPROVED

AHPatel
9/25/2012 4:14:14 AM

Integration File: events.e
Quant Time: Sep 24 08:09:25 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Sep 21 13:01:00 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

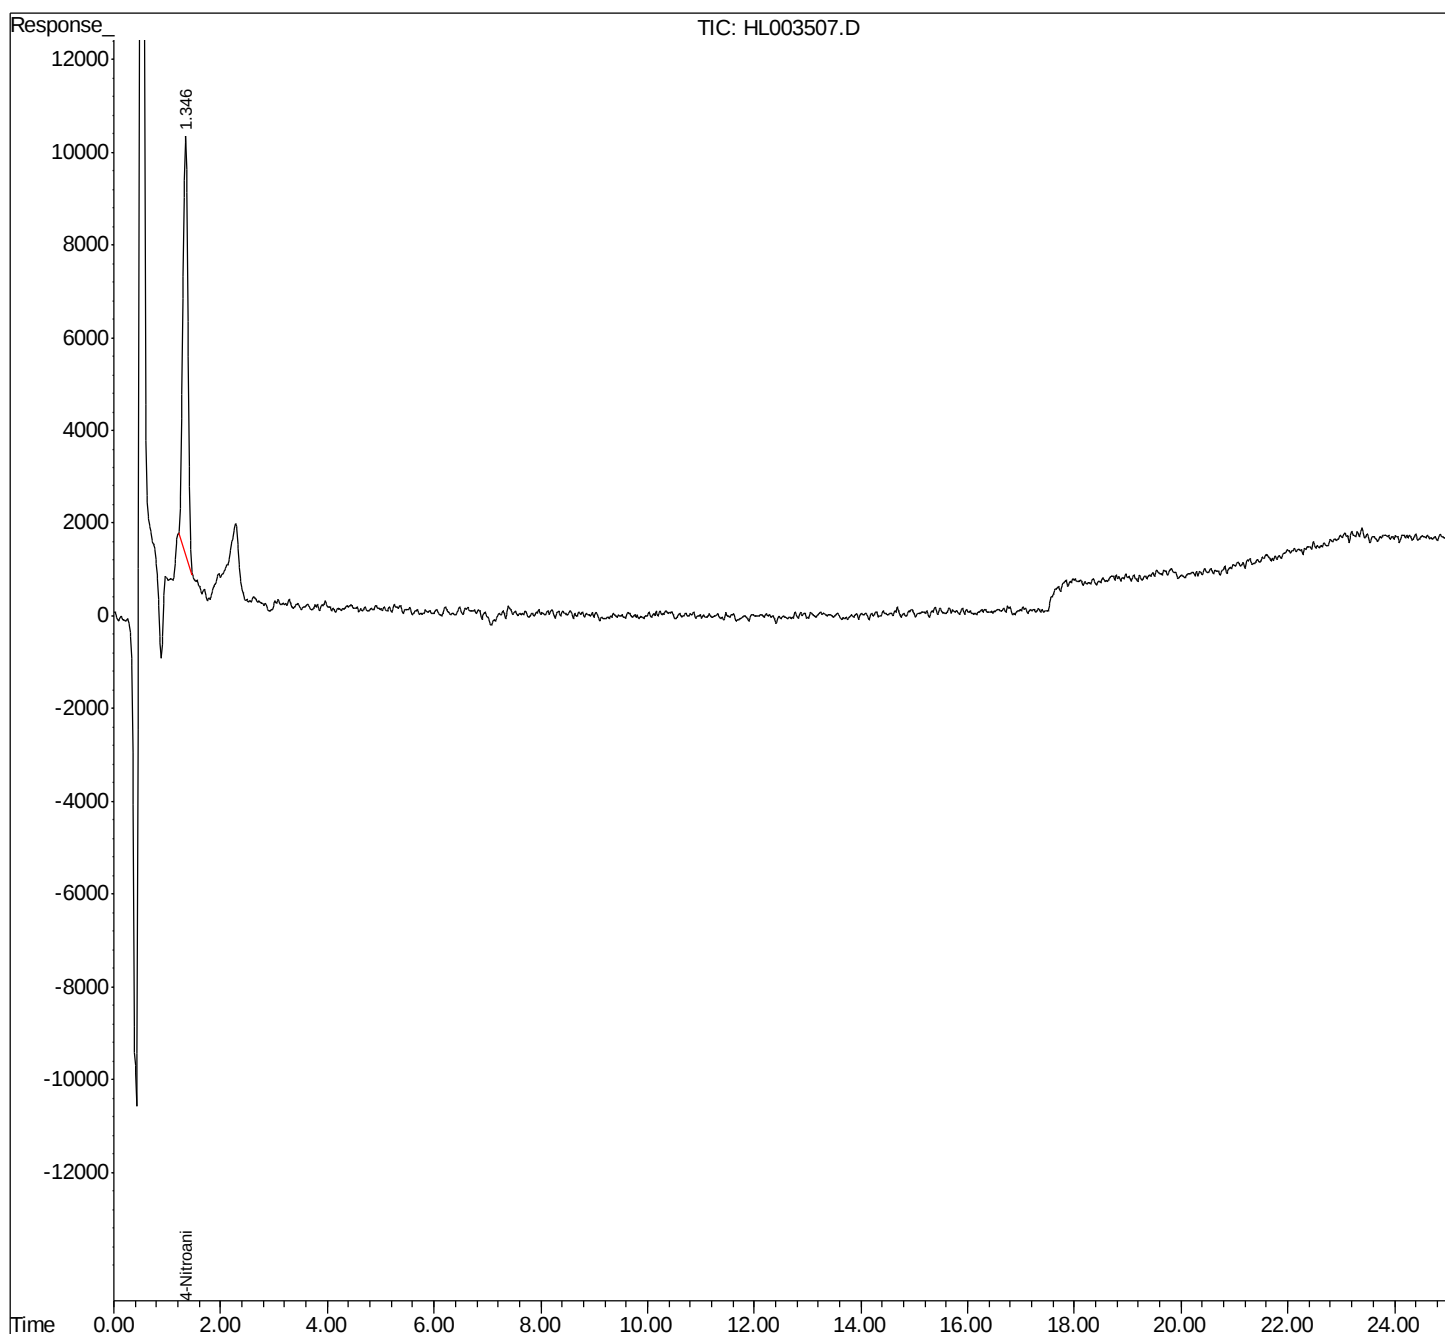

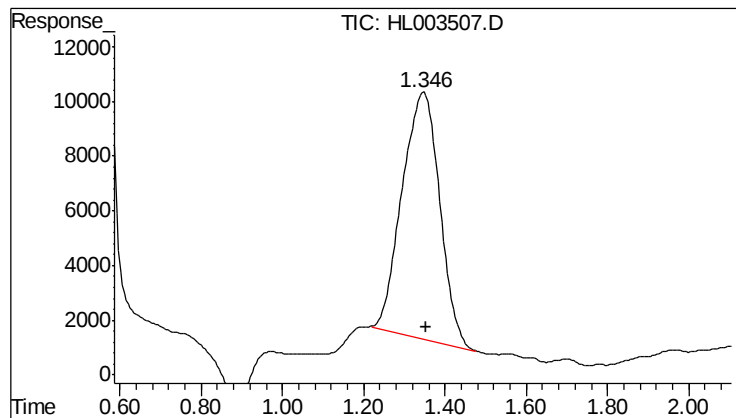

#1 4-Nitroaniline

R.T.: 1.346 min
Delta R.T.: -0.006 min
Response: 578643
Conc: 155.74 ug/L m

Instrument :
HPLC_L
ClientSampleId :
BUILDG-B3024COMP2

Manual Integrations
APPROVED

AHPatel
9/25/2012 4:14:14 AM