

Data Path : X:\HPCHEM1\HPLC\_L\Data\HL092012\  
Data File : HL003525.D  
Signal(s) : VWD1A.CH  
Acq On : 20-Sep-2012, 19:16  
Operator : HLM  
Sample : PB65783BSD2  
Misc :  
ALS Vial : 59 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
PB65783BSD2

Integration File: events.e  
Quant Time: Sep 24 08:11:58 2012  
Quant Method : H:\VOL1\HPLC\HPLC\_L\METHODS\HL091912.M  
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
QLast Update : Fri Sep 21 13:01:00 2012  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. :  
Signal Phase :  
Signal Info :

| Compound                    | R.T.           | Response | Conc Units    |
|-----------------------------|----------------|----------|---------------|
| -----                       |                |          |               |
| System Monitoring Compounds |                |          |               |
| 1) S 4-Nitroaniline         | 1.348          | 1230739  | 331.244 ug/L  |
| Spiked Amount 300.000       | Range 37 - 149 | Recovery | = 110.41%     |
|                             |                |          |               |
| Target Compounds            |                |          |               |
| 17) T Nitroglycerin         | 6.107          | 290888   | 5122.119 ug/L |
| -----                       |                |          |               |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : X:\HPCHEM1\HPLC\_L\Data\HL092012\  
Data File : HL003525.D  
Signal(s) : VWD1A.CH  
Acq On : 20-Sep-2012, 19:16  
Operator : HLM  
Sample : PB65783BSD2  
Misc :  
ALS Vial : 59 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
PB65783BSD2

Integration File: events.e  
Quant Time: Sep 24 08:11:58 2012  
Quant Method : H:\VOL1\HPLC\HPLC\_L\METHODS\HL091912.M  
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
QLast Update : Fri Sep 21 13:01:00 2012  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. :  
Signal Phase :  
Signal Info :

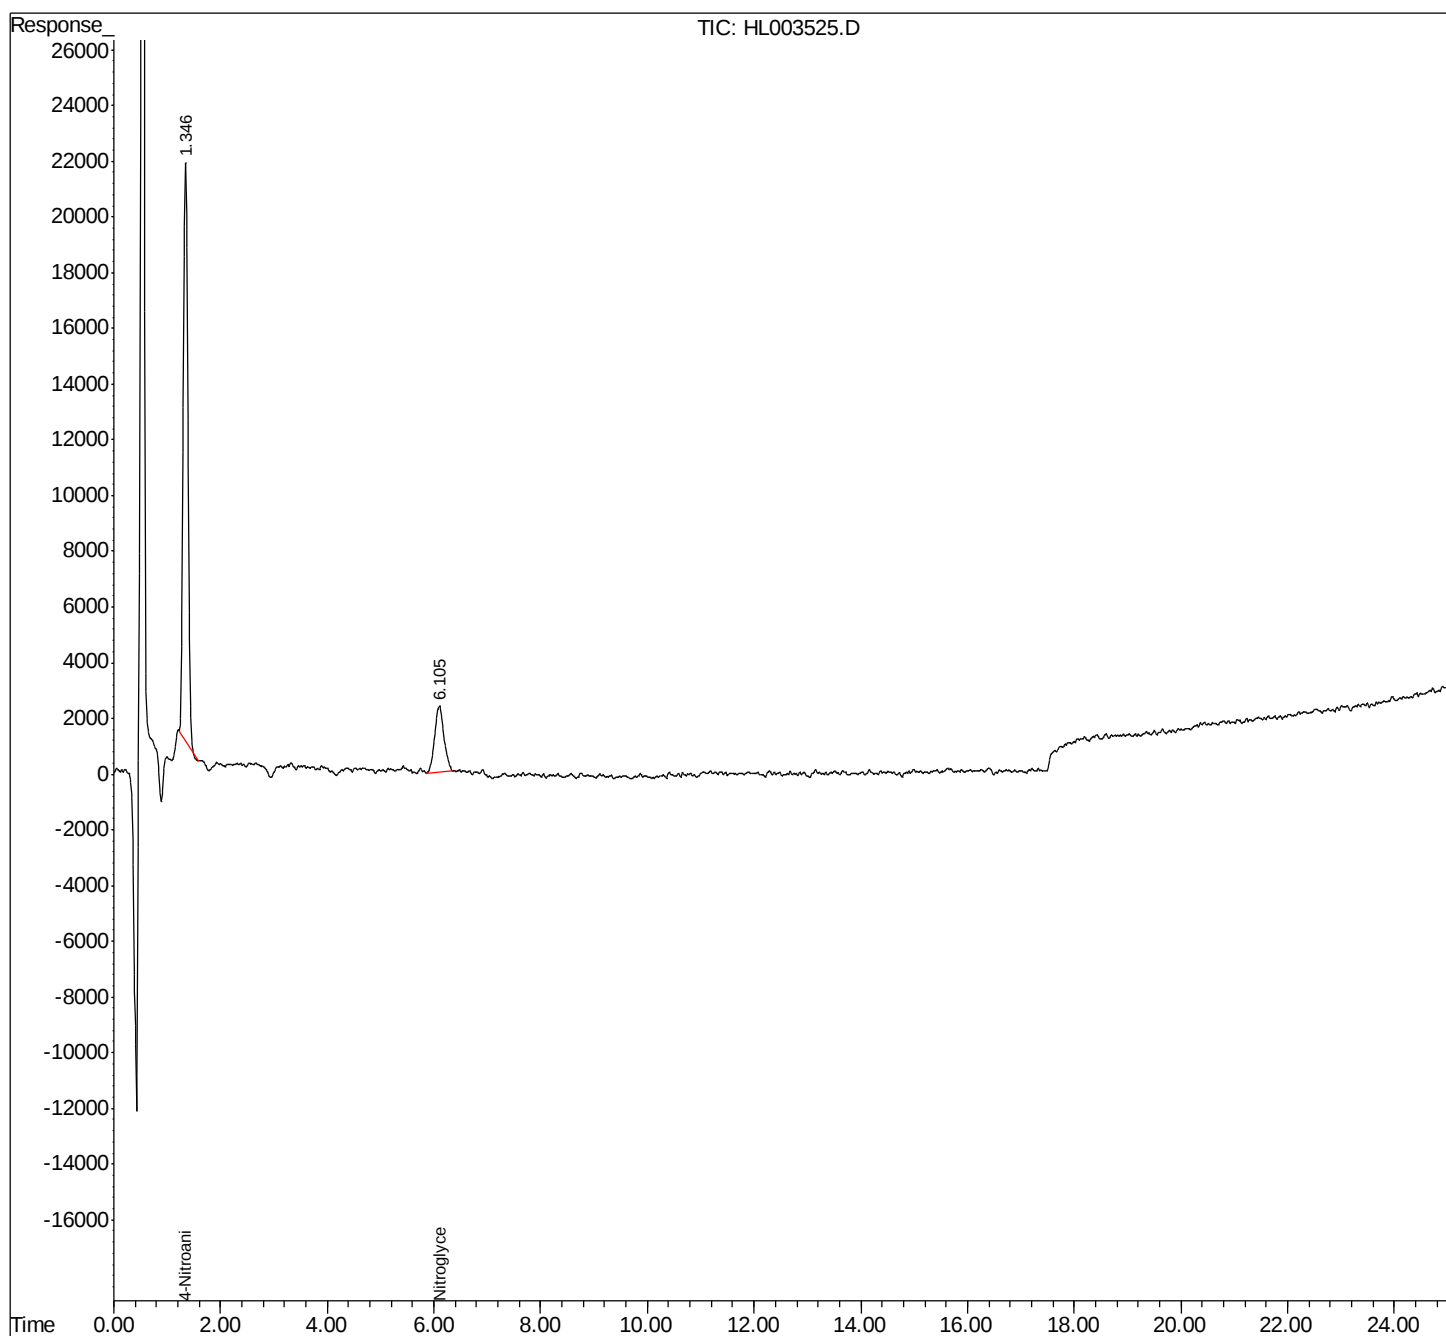


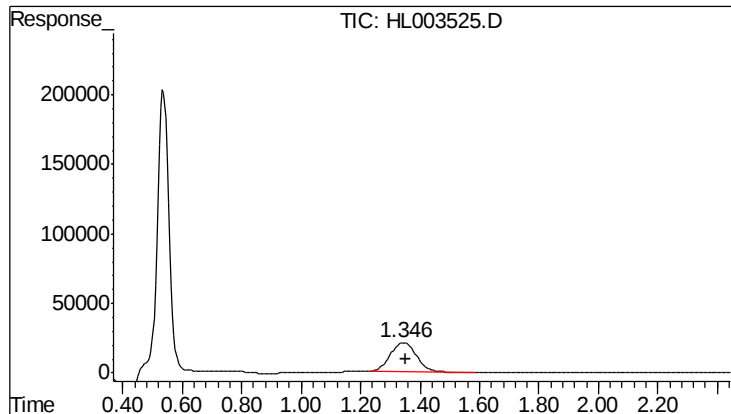

#1 4-Nitroaniline

R.T.: 1.348 min  
Delta R.T.: -0.005 min  
Response: 1230739  
Conc: 331.24 ug/L

Instrument :  
HPLC\_L  
ClientSampleId :  
PB65783BSD2

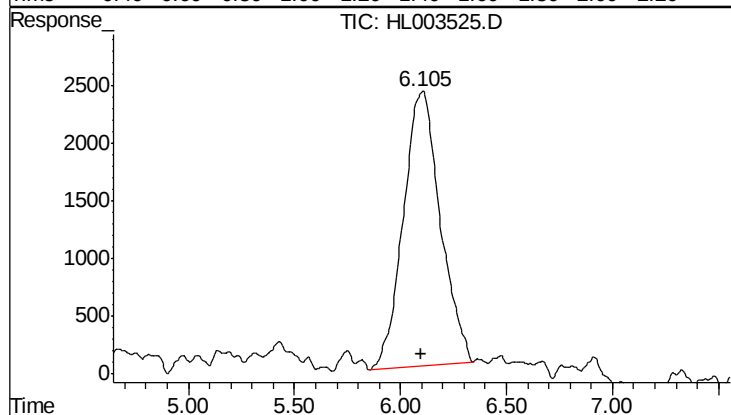

#17 Nitroglycerin

R.T.: 6.107 min  
Delta R.T.: 0.012 min  
Response: 290888  
Conc: 5122.12 ug/L