

Data File : H:\VOL1\HPLC\HPLC L\120925\HL003542.D Vial: 50
Acq On : 25-Sep-2012, 21:21 Operator: HLM
Sample : PB65898BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Sep 26 12:25 2012 Quant Results File: HL091912.RES

Instrument :
HPLC_L
ClientSampleId :
PB65898BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Tue Sep 25 17:44:26 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.33	671658	180.772 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 60.26%

Target Compounds

5) T	Tetryl	6.00	121144	14.194 ug/L
17) T	Nitroglycerin	6.00	121144	2133.172 ug/L
18) T	PETN	18.27f	8124	0.840 ug/L


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\120925\HL003542.D Vial: 50
 Acq On : 25-Sep-2012, 21:21 Operator: HLM
 Sample : PB65898BS2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Sep 26 12:25 2012 Quant Results File: HL091912.RES

Instrument :
 HPLC_L
 ClientSampleId :
 PB65898BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL091912.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Tue Sep 25 17:44:26 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

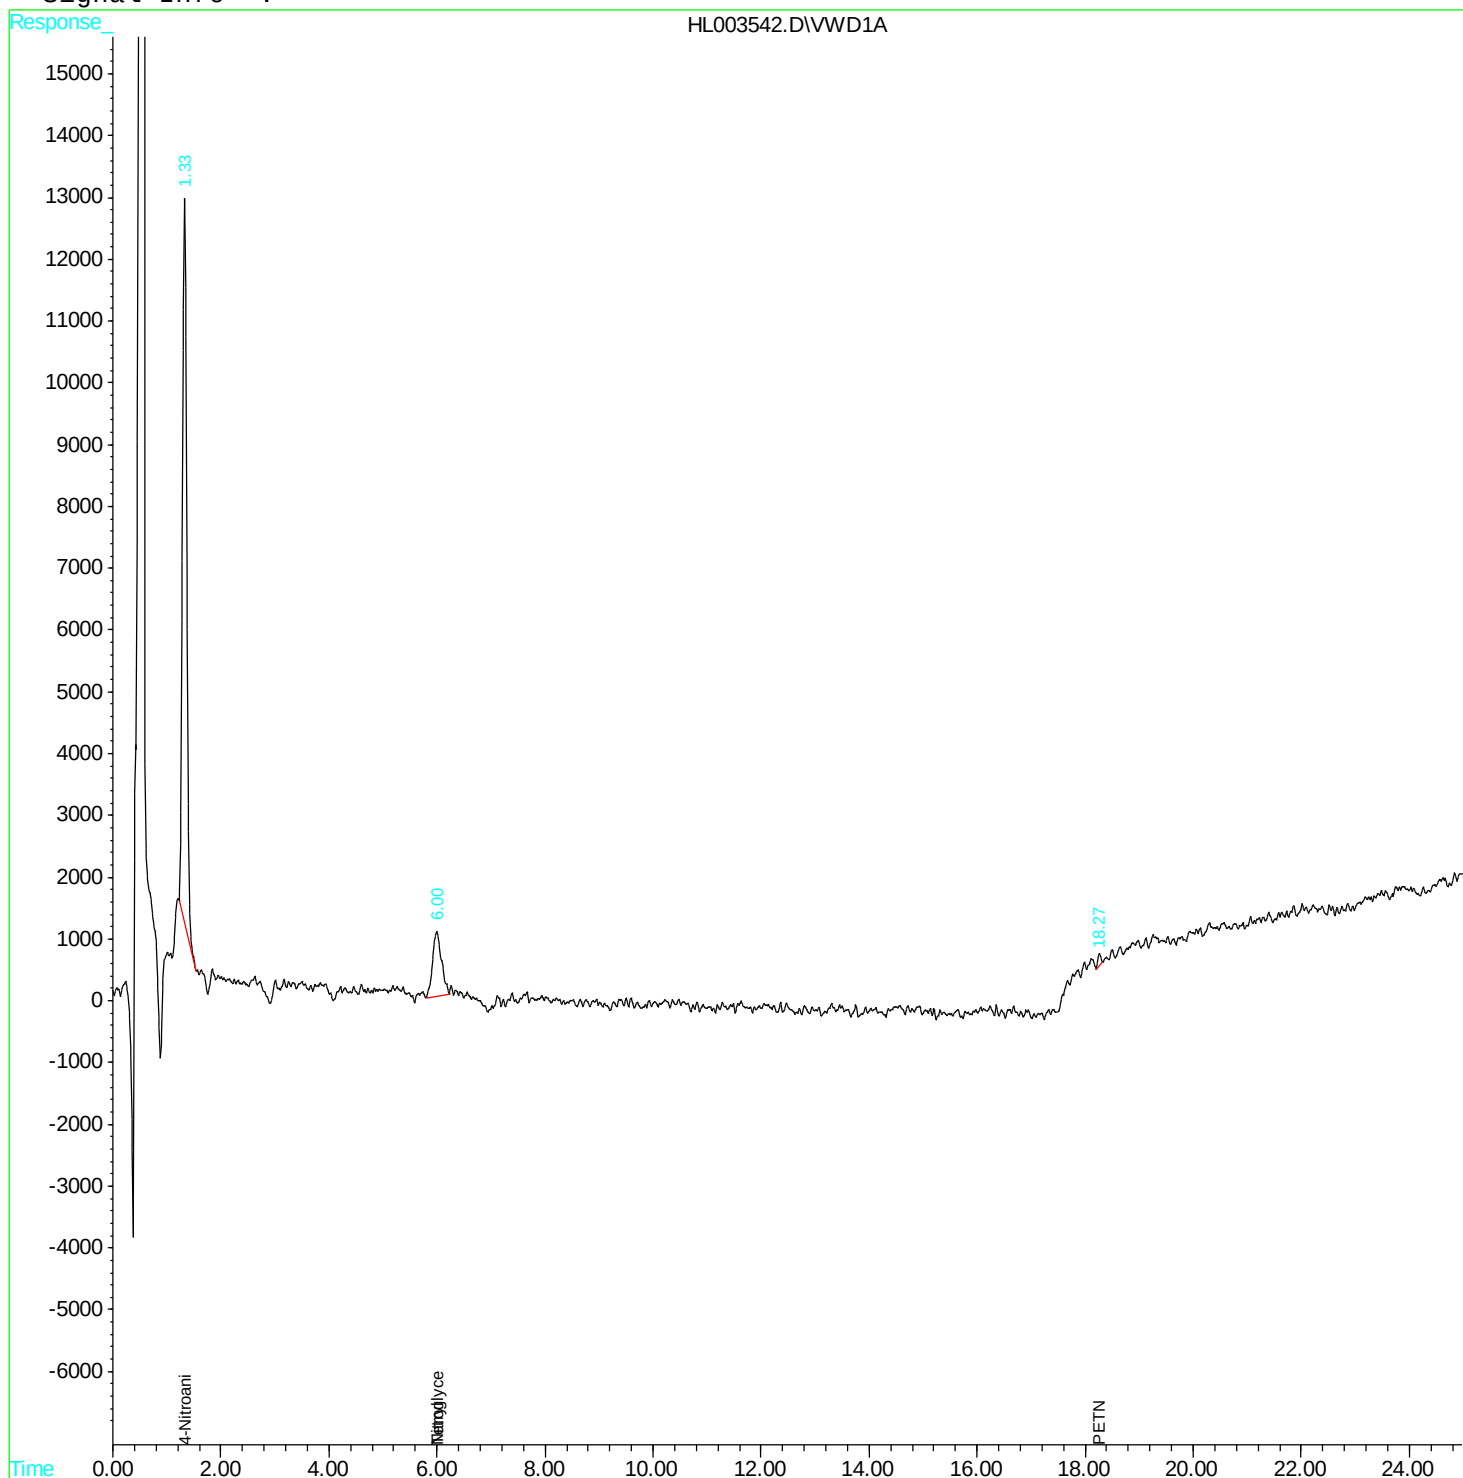


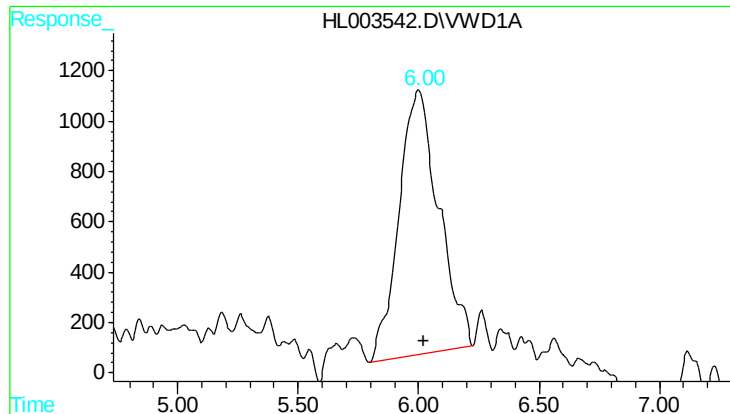

#5 Tetryl


R.T.: 6.002 min
Delta R.T.: -0.020 min
Response: 121144
Conc: 14.19 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB65898BS2

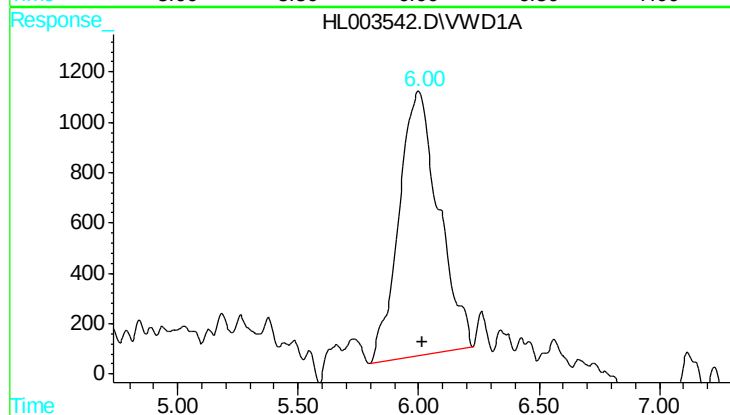

#17 Nitroglycerin

R.T.: 6.002 min
Delta R.T.: -0.015 min
Response: 121144
Conc: 2133.17 ug/L

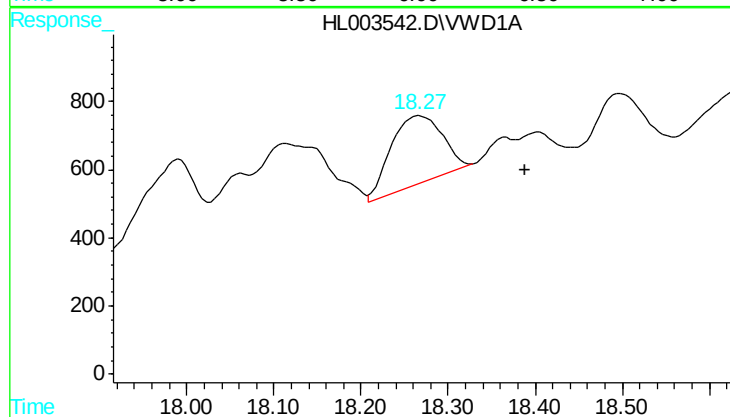

#18 PETN

R.T.: 18.268 min
Delta R.T.: -0.120 min
Response: 8124
Conc: 0.84 ug/L