

Data Path : S:\HPCHEM1\HPLC_L\Data\HL092512\
 Data File : HL003531.D
 Signal(s) : VWD1A.CH
 Acq On : 25-Sep-2012, 16:25
 Operator : HLM
 Sample : 8330-CCV
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Integration File: events.e
 Quant Time: Sep 27 03:31:08 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Tue Sep 25 17:44:26 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.340	3999284	1076.376 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 358.79%#
Target Compounds			
2) T HMX	0.900	3947791	1009.165 ug/L
3) T RDX	1.726	5401337	1038.682 ug/L
4) T 1,3,5-Trinitrobenzene	2.695	6062544	499.372 ug/L
5) T Tetryl	6.024	7825585	916.887 ug/L
6) T 2,4,6-Trinitrotoluene	6.429	5748641	510.175 ug/L
7) T 2-Amino-4,6-dinitroto...	6.853	5427557	498.601 ug/L
8) T 4-Amino-2,6-dinitroto...	7.155	3630531	525.361 ug/L
9) T 2,4-Dinitrotoluene	8.020	7539002	499.459 ug/L
10) T 2,6-Dinitrotoluene	8.378	4255953	488.955 ug/L
11) T 1,3-Dinitrobenzene	3.564	8106527	511.690 ug/L
12) T Nitrobenzene	4.782	5316351	517.084 ug/L
13) T 2-Nitrotoluene	11.556	6489145	984.004 ug/L
14) T 3-Nitrotoluene	13.536	6862343	970.324 ug/L
15) T 4-Nitrotoluene	12.299	5492360	995.022 ug/L
16) T 3,5-Dinitroaniline	3.879	15263806	998.027 ug/L
18) T PETN	18.388	22181851	2292.681 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL092512\
Data File : HL003531.D
Signal(s) : VWD1A.CH
Acq On : 25-Sep-2012, 16:25
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Sep 27 03:31:08 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Tue Sep 25 17:44:26 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

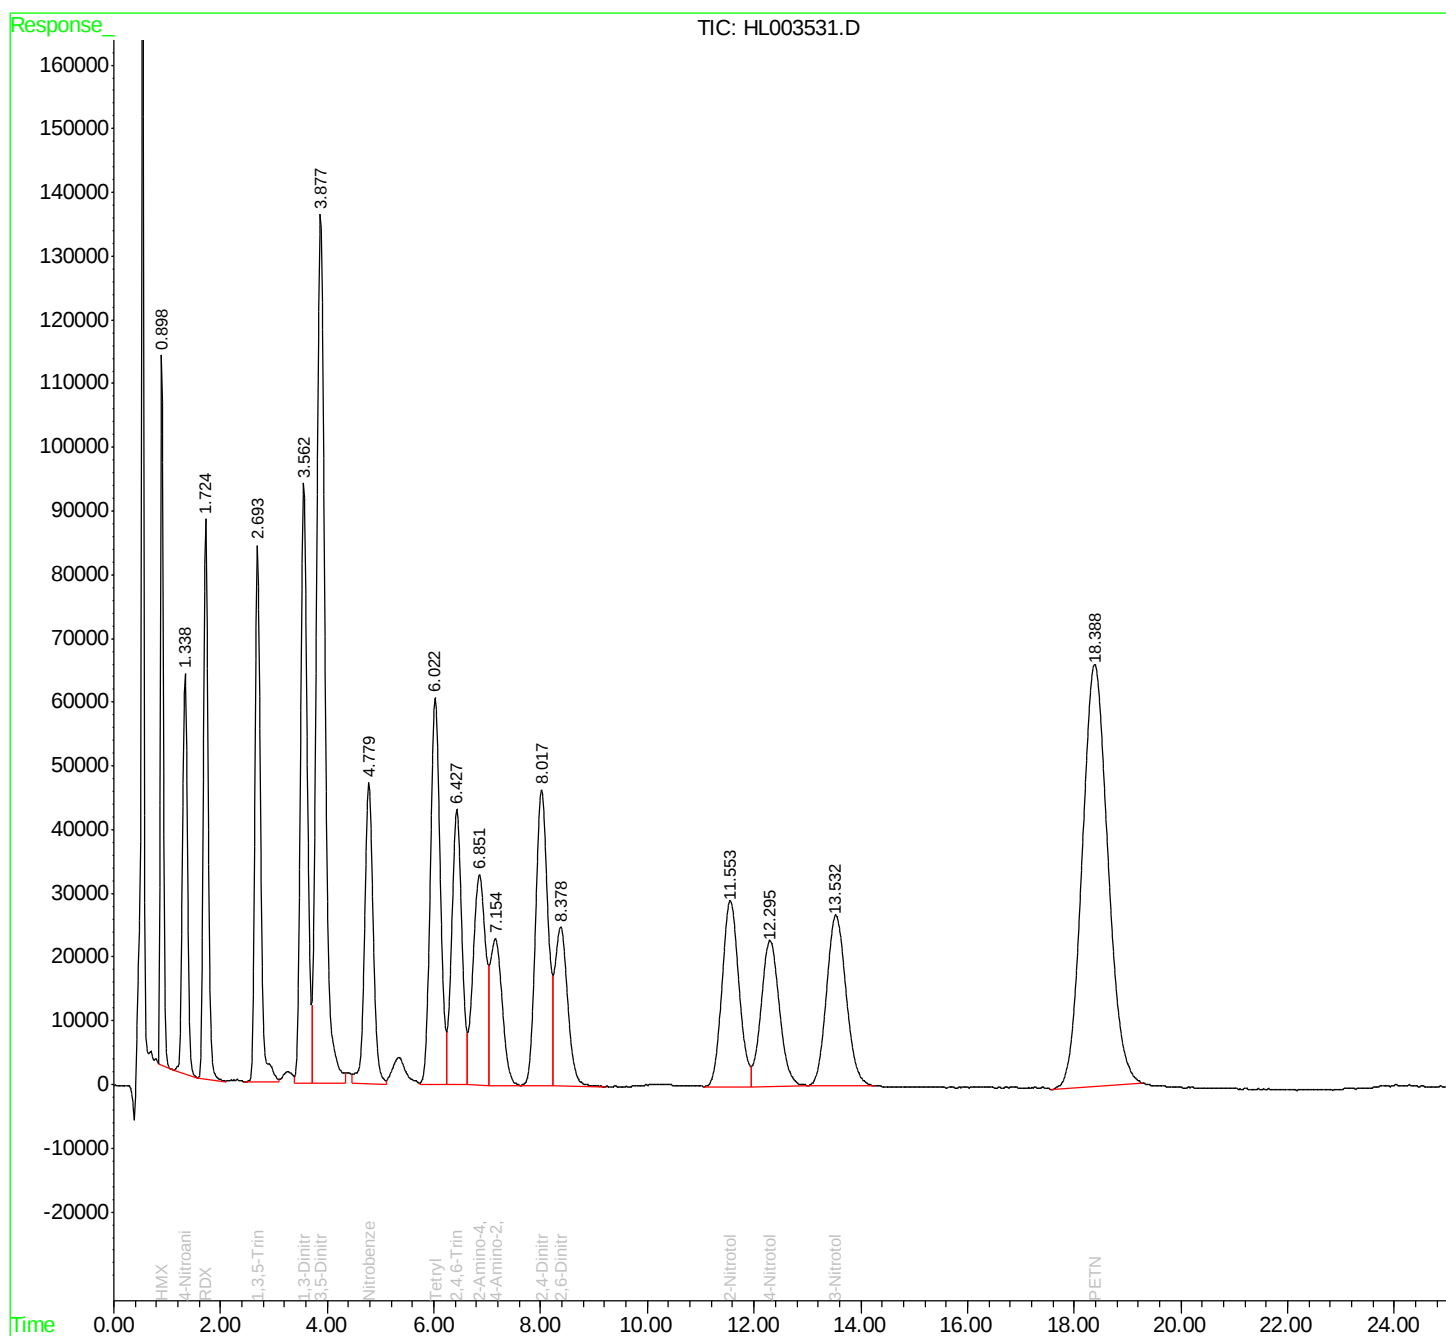


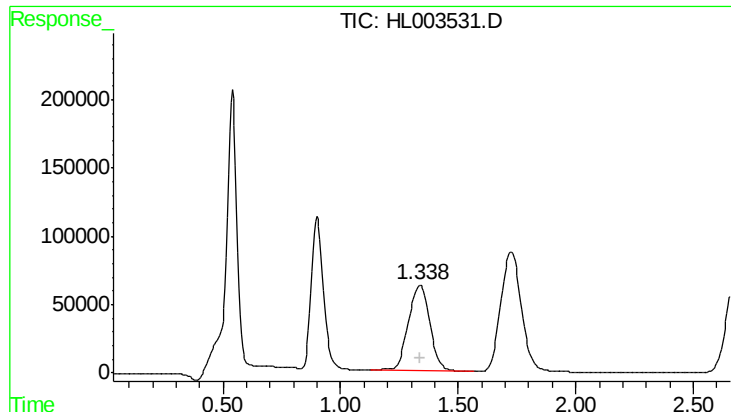

#1 4-Nitroaniline


R.T.: 1.340 min
Delta R.T.: 0.000 min
Response: 3999284
Conc: 1076.38 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

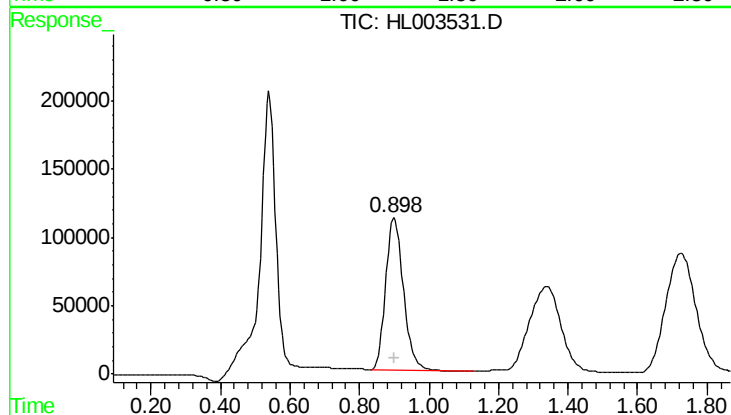


#2 HMX

R.T.: 0.900 min
Delta R.T.: 0.000 min
Response: 3947791
Conc: 1009.17 ug/L

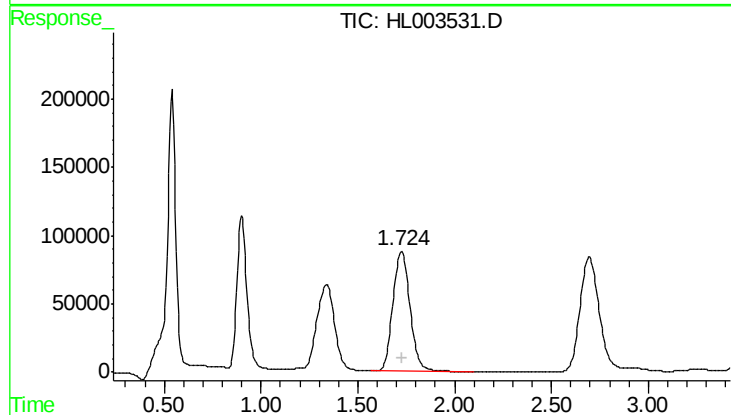


#3 RDX

R.T.: 1.726 min
Delta R.T.: 0.000 min
Response: 5401337
Conc: 1038.68 ug/L

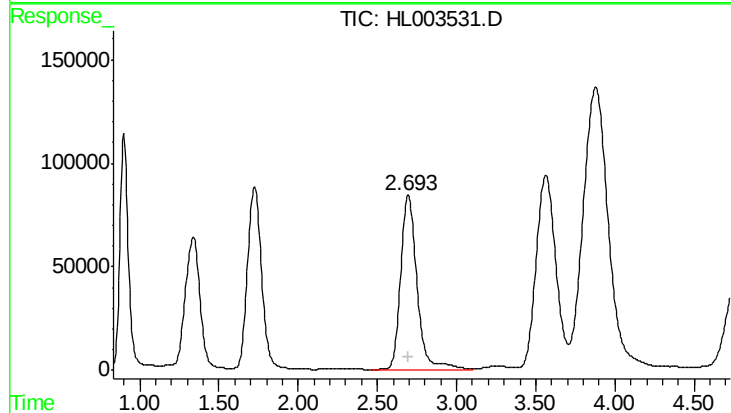

#4 1,3,5-Trinitrobenzene


R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 6062544
Conc: 499.37 ug/L

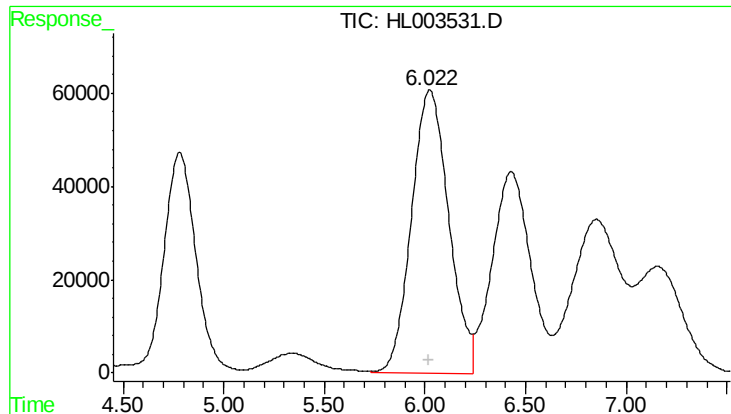

#5 Tetryl


R.T.: 6.024 min
Delta R.T.: 0.002 min
Response: 7825585
Conc: 916.89 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

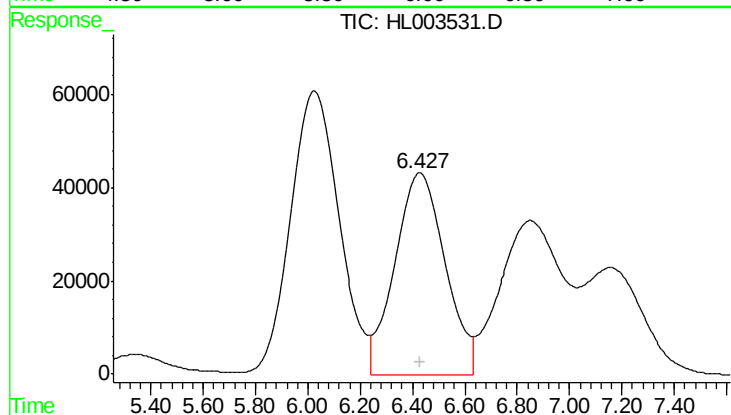


#6 2,4,6-Trinitrotoluene

R.T.: 6.429 min
Delta R.T.: 0.002 min
Response: 5748641
Conc: 510.17 ug/L

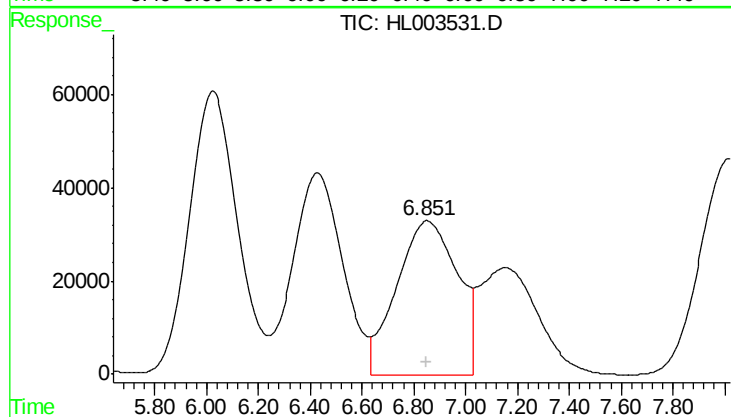


#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.853 min
Delta R.T.: 0.002 min
Response: 5427557
Conc: 498.60 ug/L

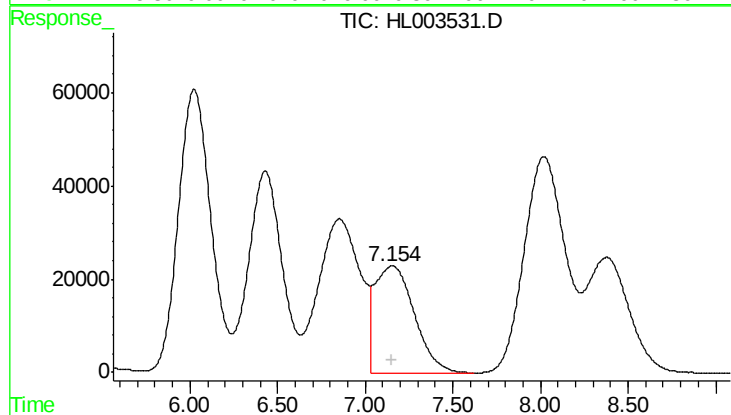

#8 4-Amino-2,6-dinitrotoluene


R.T.: 7.155 min
Delta R.T.: 0.002 min
Response: 3630531
Conc: 525.36 ug/L

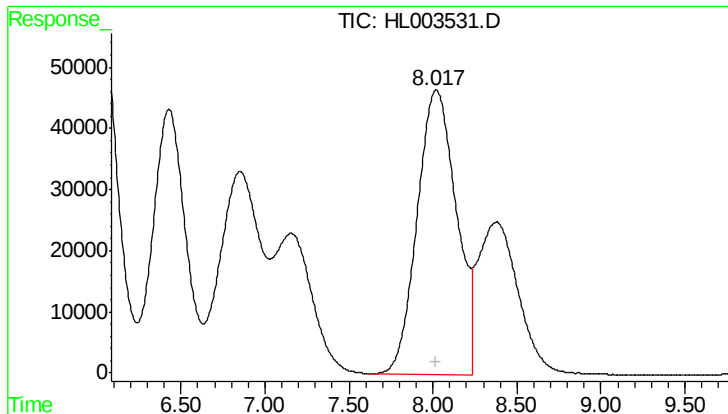

#9 2,4-Dinitrotoluene


R.T.: 8.020 min
Delta R.T.: 0.002 min
Response: 7539002
Conc: 499.46 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

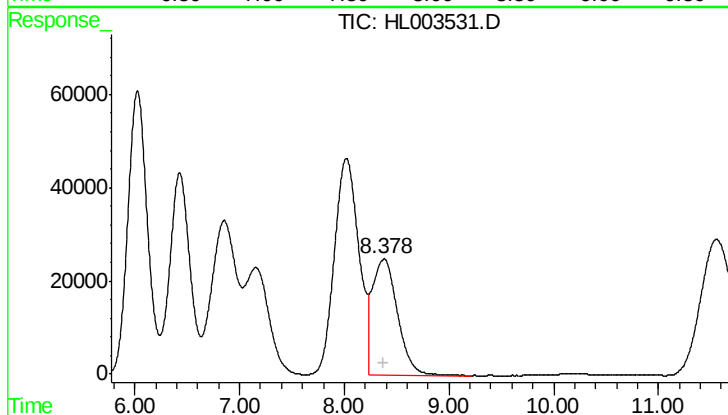


#10 2,6-Dinitrotoluene

R.T.: 8.378 min
Delta R.T.: 0.000 min
Response: 4255953
Conc: 488.95 ug/L

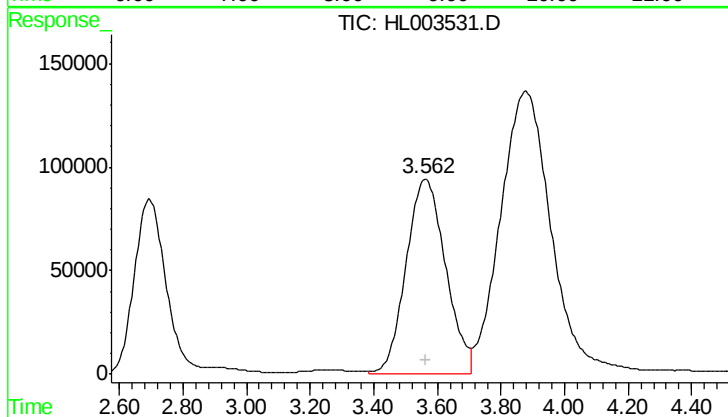


#11 1,3-Dinitrobenzene

R.T.: 3.564 min
Delta R.T.: 0.002 min
Response: 8106527
Conc: 511.69 ug/L

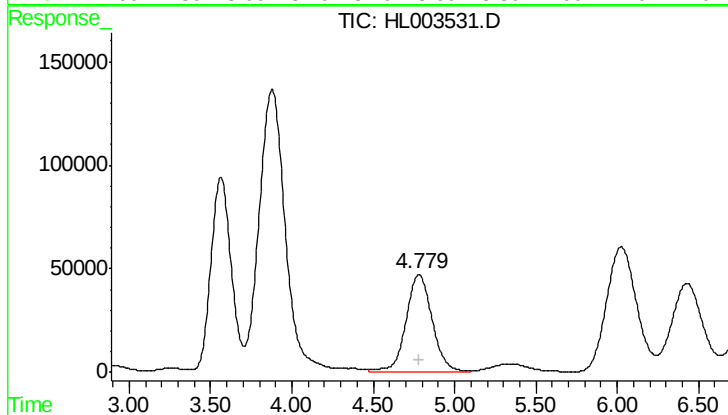

#12 Nitrobenzene


R.T.: 4.782 min
Delta R.T.: 0.002 min
Response: 5316351
Conc: 517.08 ug/L

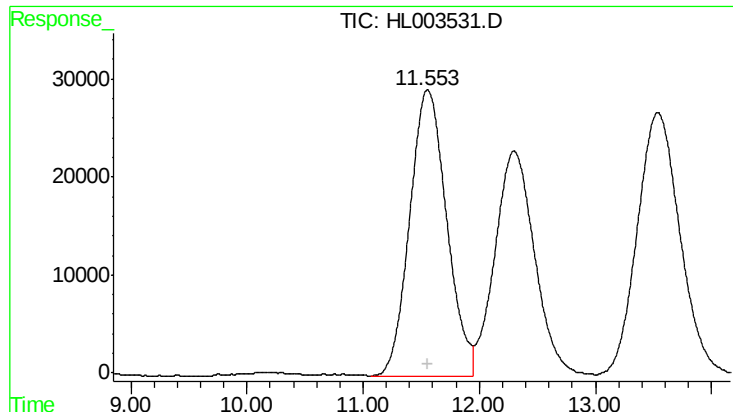

#13 2-Nitrotoluene


R.T.: 11.556 min
Delta R.T.: 0.002 min
Response: 6489145
Conc: 984.00 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

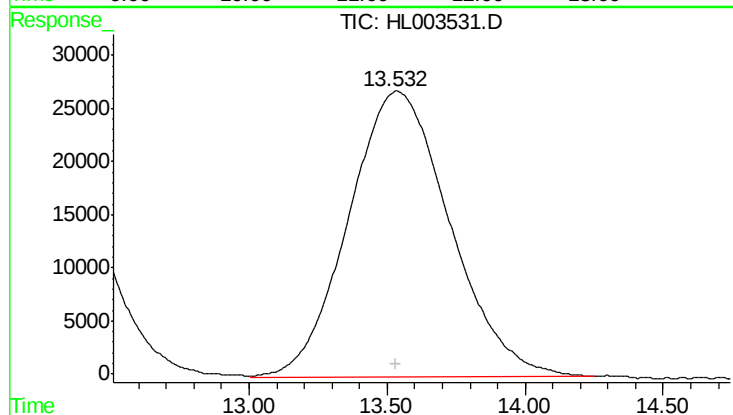


#14 3-Nitrotoluene

R.T.: 13.536 min
Delta R.T.: 0.004 min
Response: 6862343
Conc: 970.32 ug/L

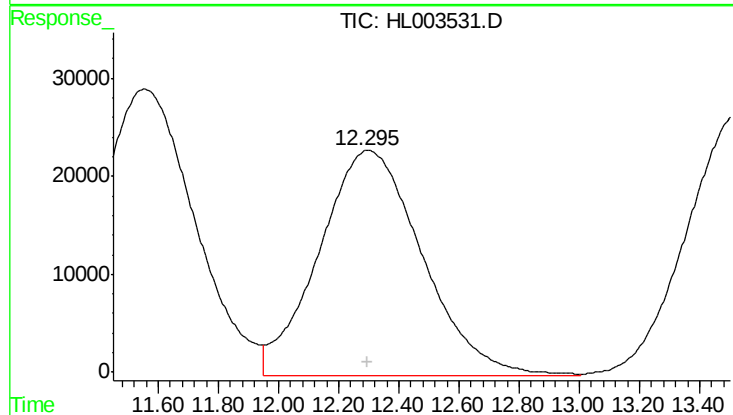


#15 4-Nitrotoluene

R.T.: 12.299 min
Delta R.T.: 0.004 min
Response: 5492360
Conc: 995.02 ug/L

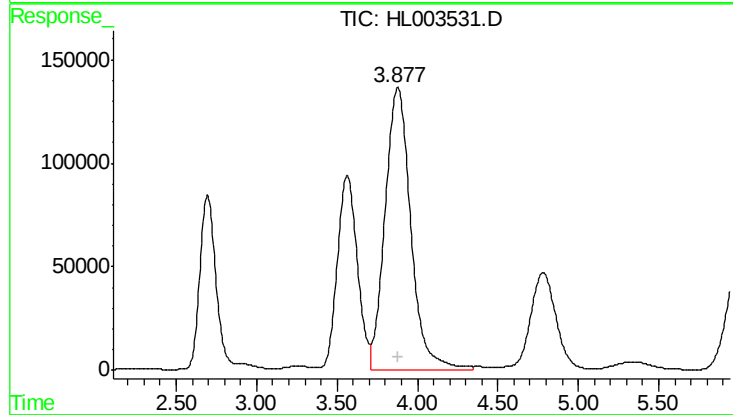

#16 3,5-Dinitroaniline

R.T.: 3.879 min
Delta R.T.: 0.000 min
Response: 15263806
Conc: 998.03 ug/L

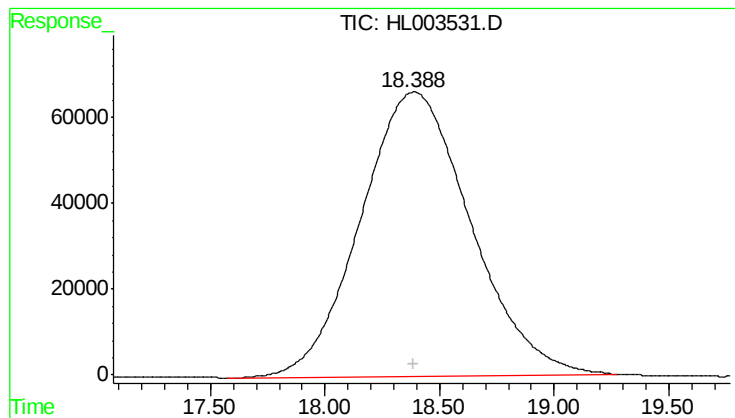

#18 PETN

R.T.: 18.388 min
Delta R.T.: 0.000 min
Response: 22181851
Conc: 2292.68 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV