

Data Path : S:\HPCHEM1\HPLC_L\Data\HL092612\
Data File : HL003569.D
Signal(s) : VWD1A.CH
Acq On : 26-Sep-2012, 22:04
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Sep 29 05:49:10 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Sep 20 08:22:23 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.366f	3985707	1072.722 ug/L
Spiked Amount 300.000 Range	37 - 149	Recovery	= 357.57%#
Target Compounds			
2) T HMX	0.915f	4071056	1040.676 ug/L
3) T RDX	1.762f	5496997	1057.077 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL092612\
Data File : HL003569.D
Signal(s) : VWD1A.CH
Acq On : 26-Sep-2012, 22:04
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Sep 29 05:49:10 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Sep 20 08:22:23 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

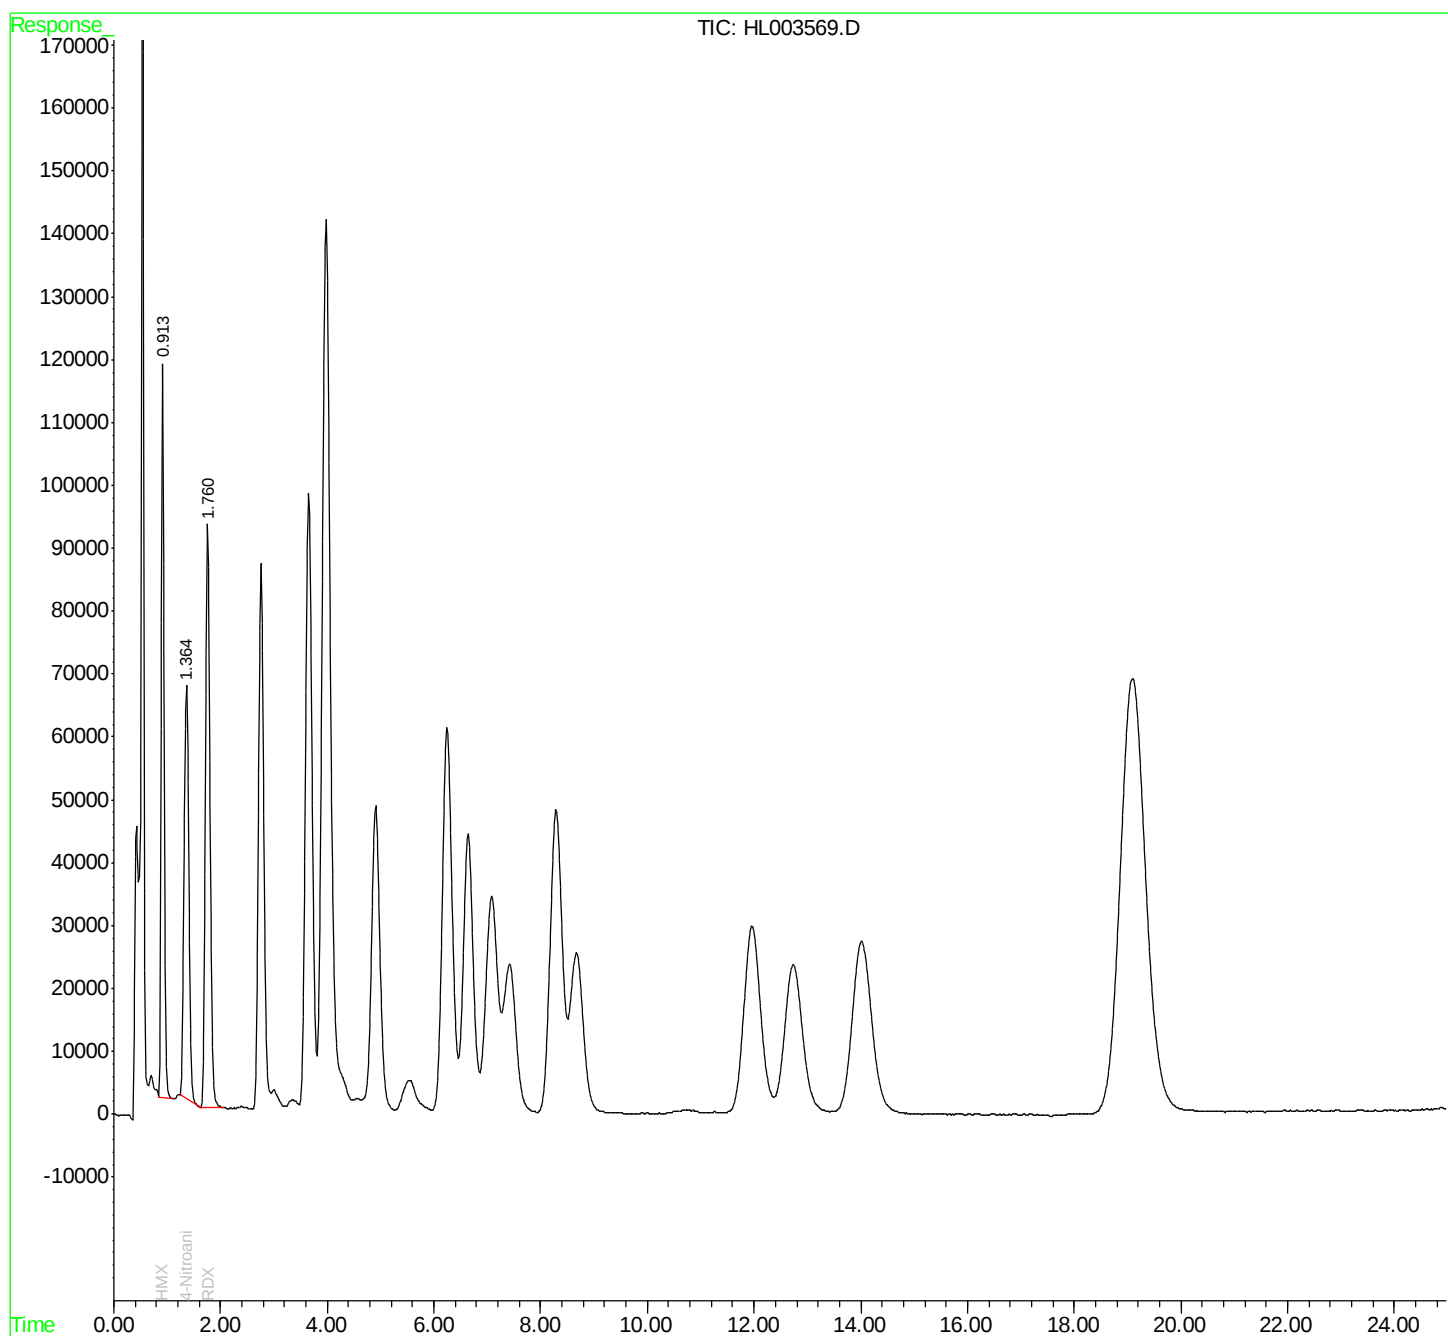


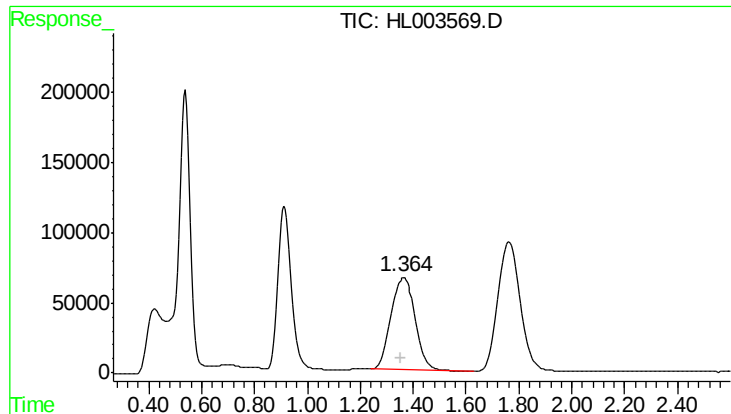

#1 4-Nitroaniline


R.T.: 1.366 min
Delta R.T.: 0.014 min
Response: 3985707
Conc: 1072.72 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

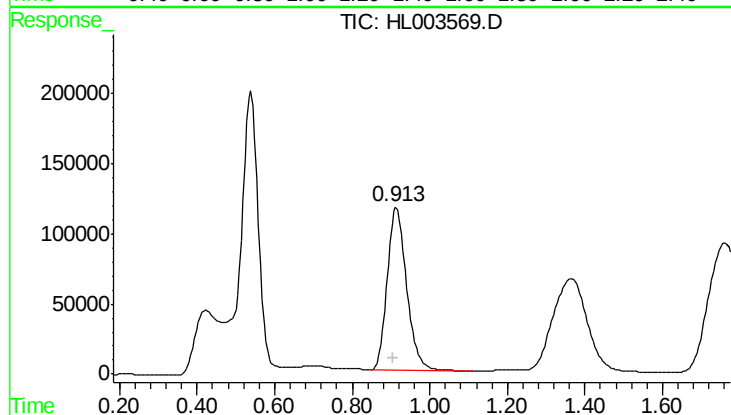

#2 HMX

R.T.: 0.915 min
Delta R.T.: 0.008 min
Response: 4071056
Conc: 1040.68 ug/L

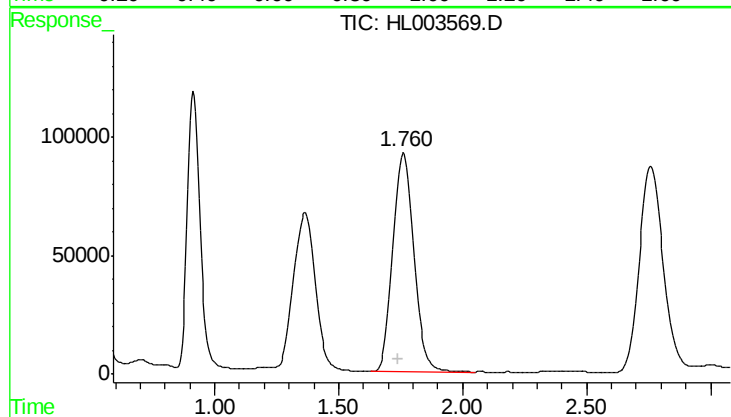

#3 RDX

R.T.: 1.762 min
Delta R.T.: 0.019 min
Response: 5496997
Conc: 1057.08 ug/L