

Data Path : S:\HPCHEM1\HPLC_L\Data\HL092612\
Data File : HL003576.D
Signal(s) : VWD1A.CH
Acq On : 27-Sep-2012, 01:13
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Sep 29 05:50:01 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Sep 20 08:22:23 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.364	4008175	1078.769 ug/L
Spiked Amount 300.000 Range	37 - 149	Recovery	= 359.59%#
Target Compounds			
2) T HMX	0.913	4096612	1047.208 ug/L
3) T RDX	1.759f	5521689	1061.826 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL092612\
Data File : HL003576.D
Signal(s) : VWD1A.CH
Acq On : 27-Sep-2012, 01:13
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Sep 29 05:50:01 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Sep 20 08:22:23 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

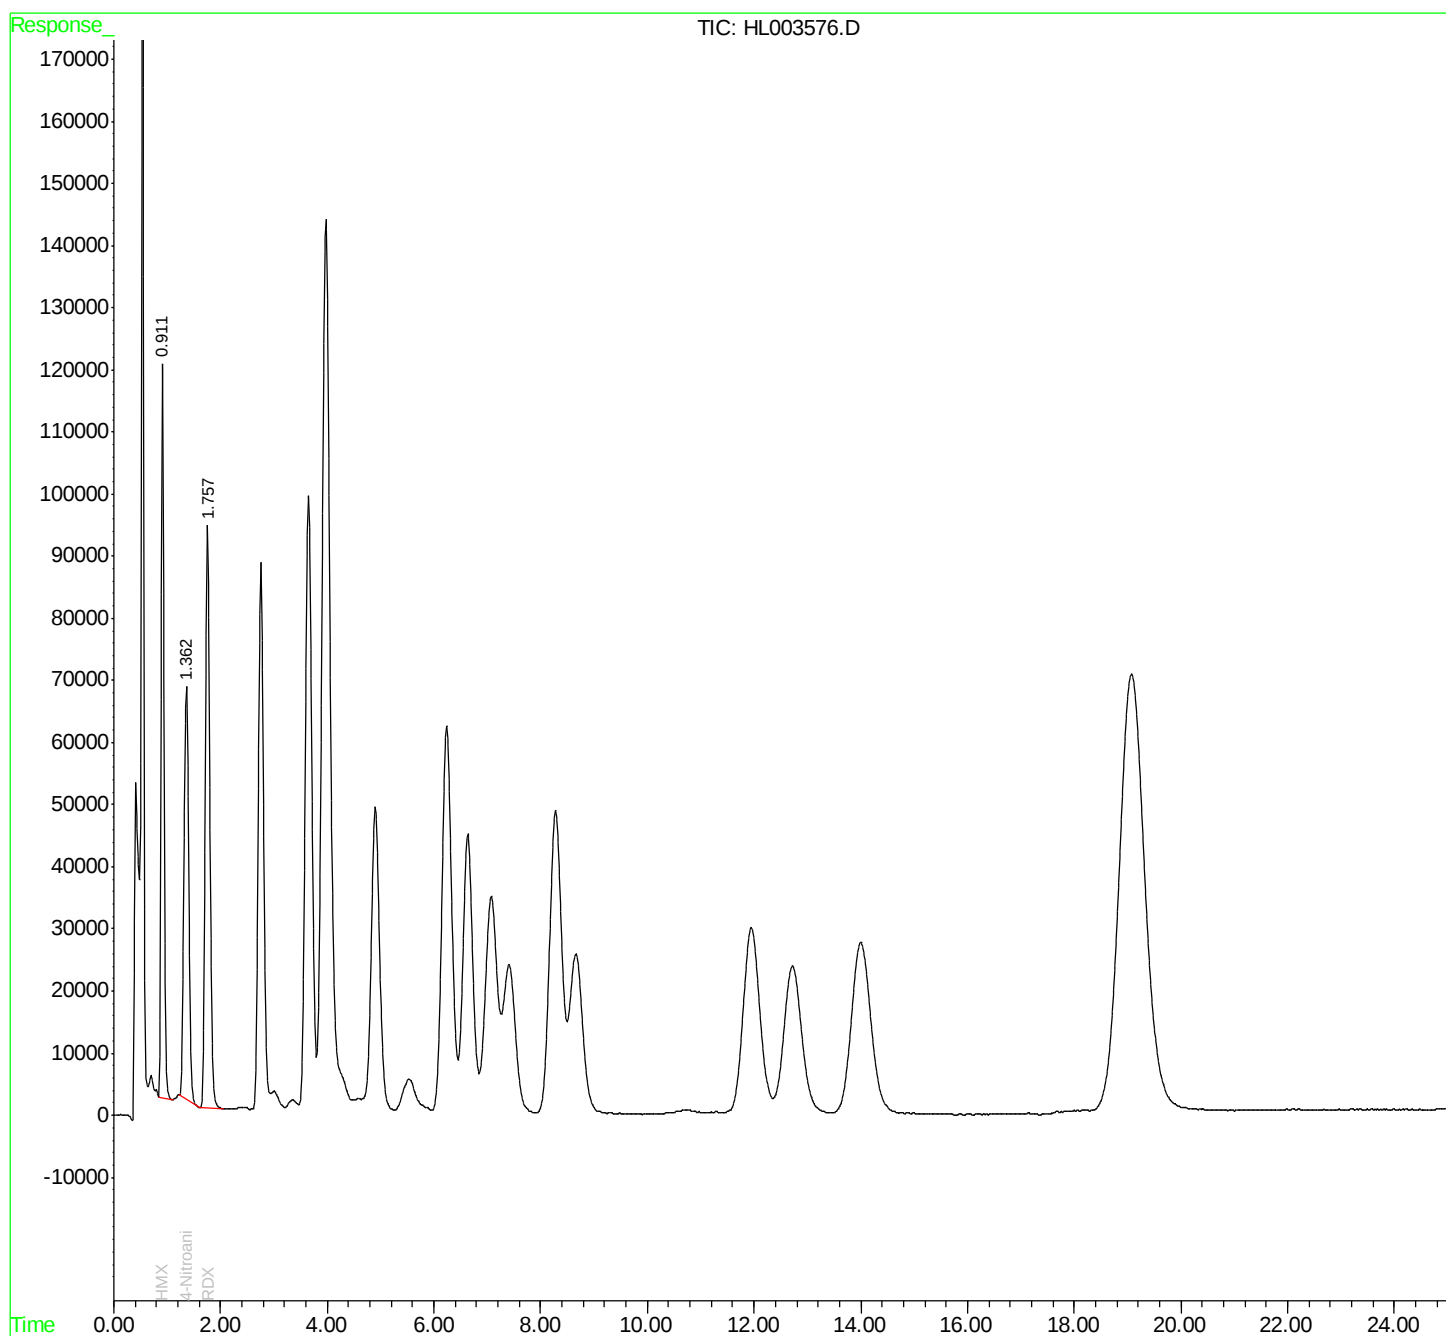


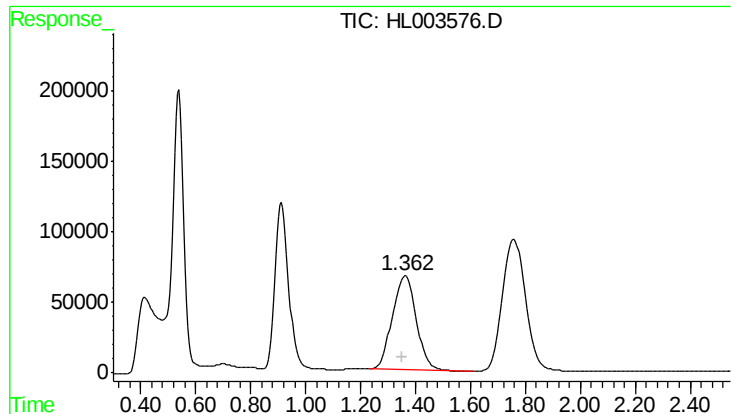

#1 4-Nitroaniline


R.T.: 1.364 min
Delta R.T.: 0.012 min
Response: 4008175
Conc: 1078.77 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

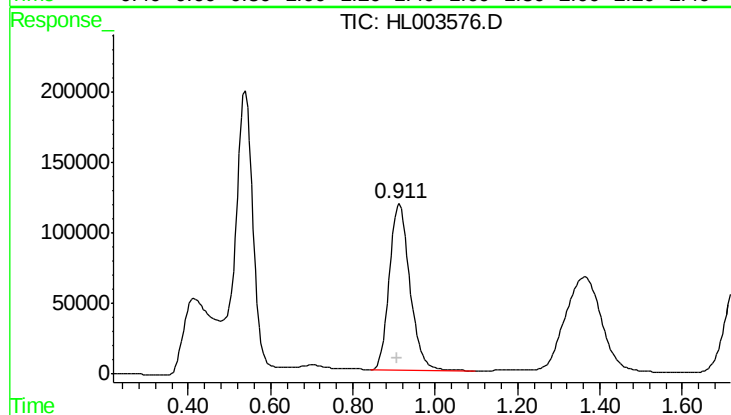

#2 HMX

R.T.: 0.913 min
Delta R.T.: 0.006 min
Response: 4096612
Conc: 1047.21 ug/L

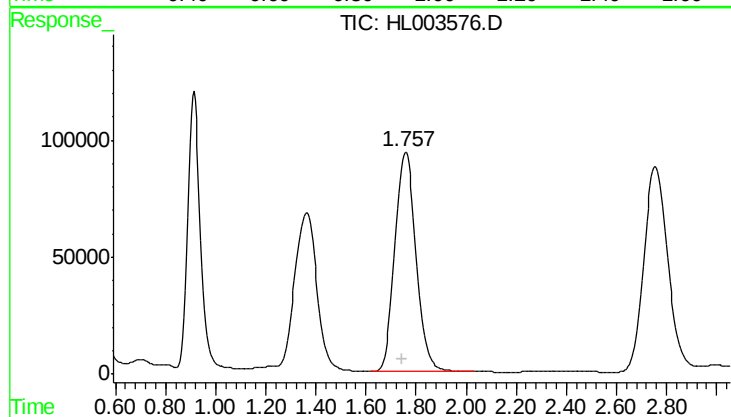

#3 RDX

R.T.: 1.759 min
Delta R.T.: 0.017 min
Response: 5521689
Conc: 1061.83 ug/L