

Data Path : S:\HPCHEM1\HPLC_L\Data\HL092612\
 Data File : HL003576.D
 Signal(s) : VWD1A.CH
 Acq On : 27-Sep-2012, 01:13
 Operator : HLM
 Sample : 8330-CCV
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Integration File: events.e
 Quant Time: Sep 29 05:43:27 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Fri Sep 28 11:30:45 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.364	4008175	1078.769 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 359.59%#
Target Compounds			
2) T HMX	0.913	4096612	1047.208 ug/L
3) T RDX	1.759	5521689	1061.826 ug/L
4) T 1,3,5-Trinitrobenzene	2.757	5889997	485.160 ug/L
5) T Tetryl	6.241	7898817	925.468 ug/L
6) T 2,4,6-Trinitrotoluene	6.635	5812065	515.803 ug/L
7) T 2-Amino-4,6-dinitroto...	7.077	5492666	504.582 ug/L
8) T 4-Amino-2,6-dinitroto...	7.408	3808940	551.178 ug/L
9) T 2,4-Dinitrotoluene	8.280	7709974	510.786 ug/L
10) T 2,6-Dinitrotoluene	8.663	4355972	500.446 ug/L
11) T 1,3-Dinitrobenzene	3.650	8317416	525.001 ug/L
12) T Nitrobenzene	4.904	5447845	529.873 ug/L
13) T 2-Nitrotoluene	11.949	6602302	1001.163 ug/L
14) T 3-Nitrotoluene	14.003	6986359	987.860 ug/L
15) T 4-Nitrotoluene	12.722	5613876	1017.036 ug/L
16) T 3,5-Dinitroaniline	3.978	15896938	1039.425 ug/L
18) T PETN	19.078	23505184	2429.459 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL092612\
Data File : HL003576.D
Signal(s) : VWD1A.CH
Acq On : 27-Sep-2012, 01:13
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Sep 29 05:43:27 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL091912.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Sep 28 11:30:45 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

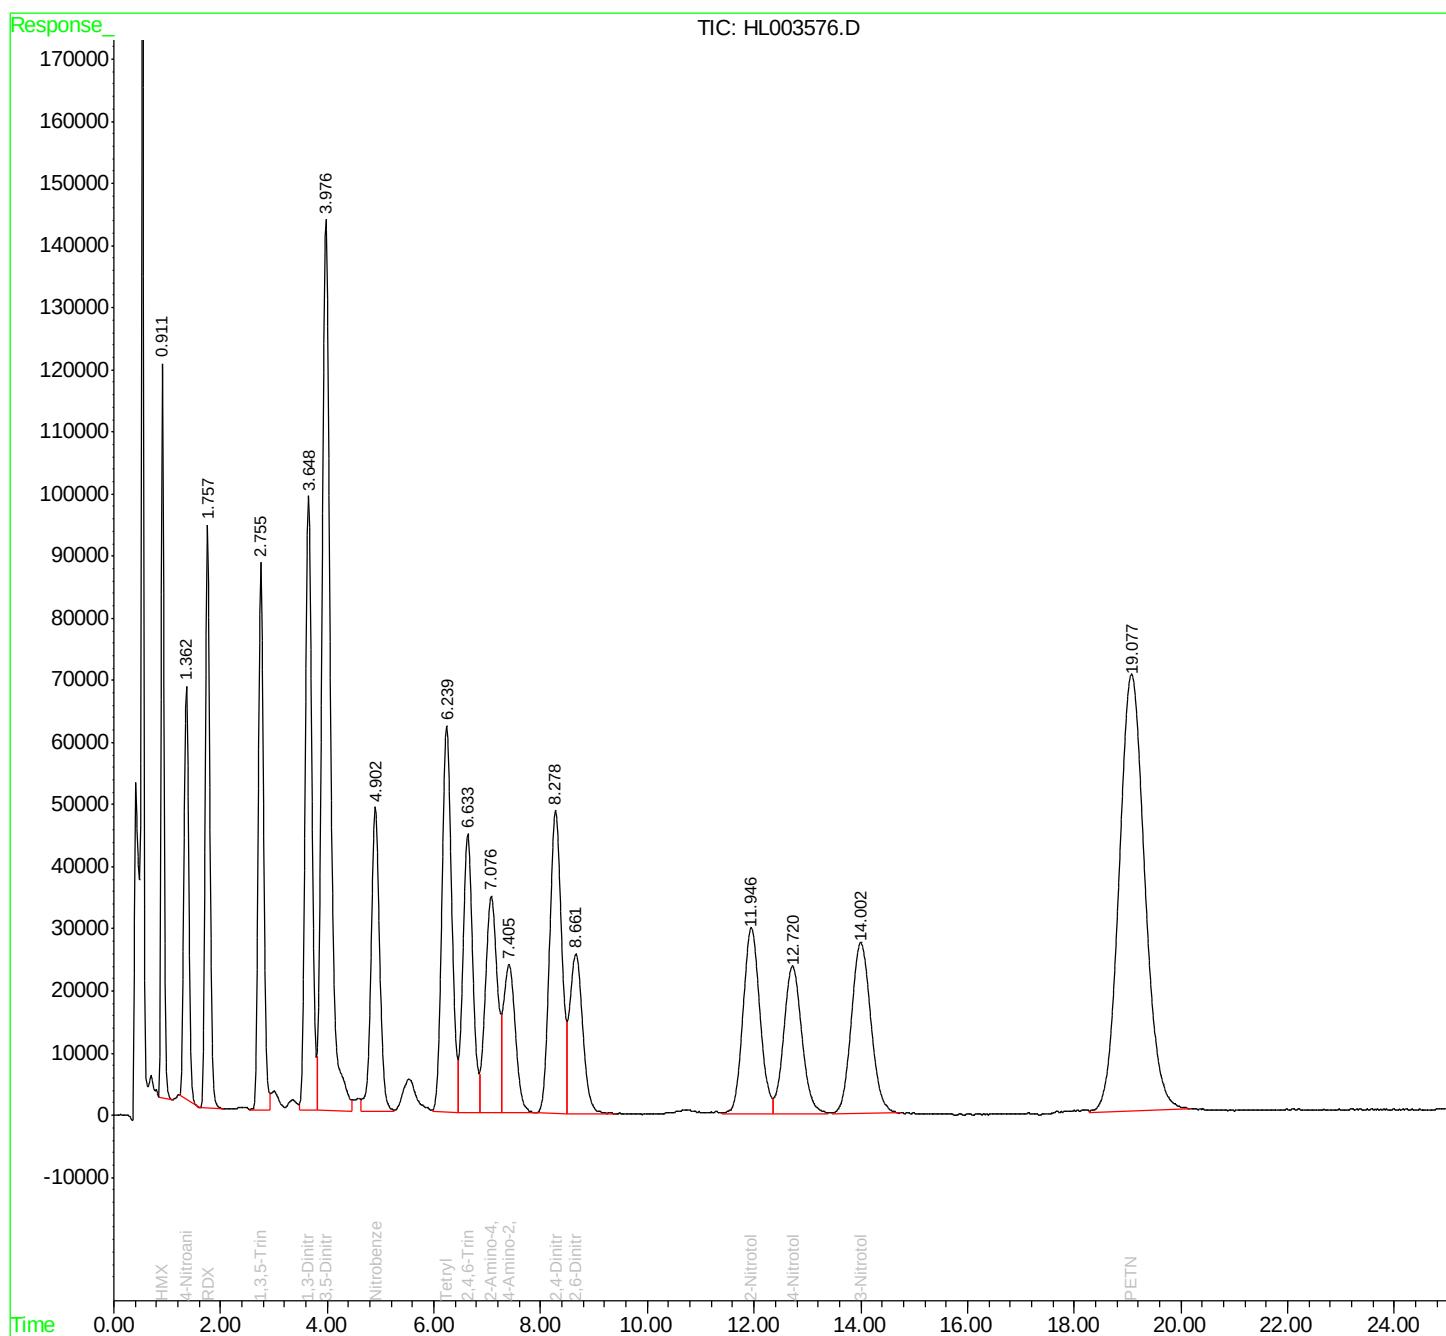


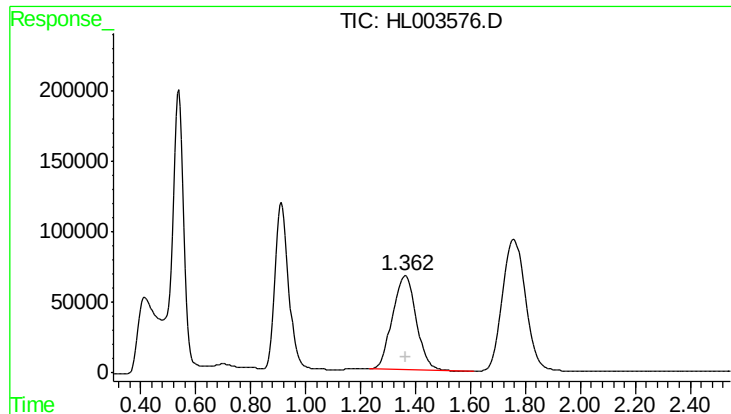

#1 4-Nitroaniline


R.T.: 1.364 min
Delta R.T.: 0.000 min
Response: 4008175
Conc: 1078.77 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

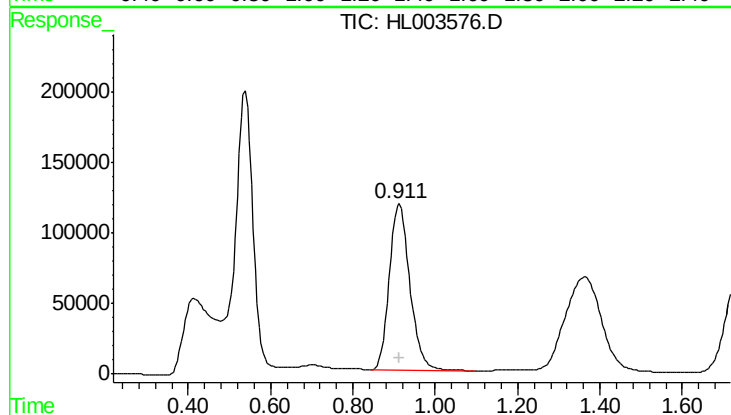


#2 HMX

R.T.: 0.913 min
Delta R.T.: 0.000 min
Response: 4096612
Conc: 1047.21 ug/L

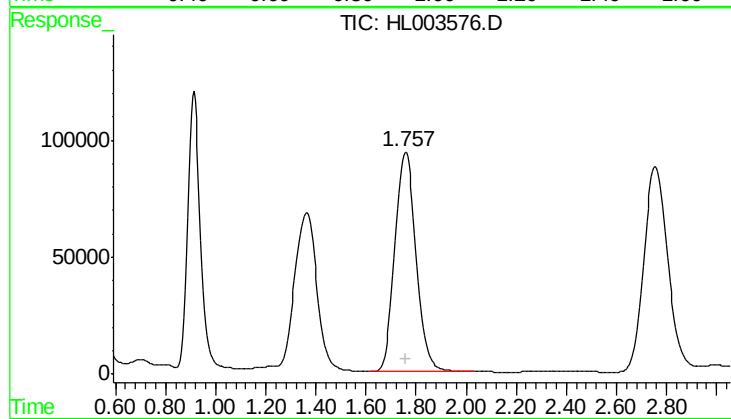


#3 RDX

R.T.: 1.759 min
Delta R.T.: 0.000 min
Response: 5521689
Conc: 1061.83 ug/L

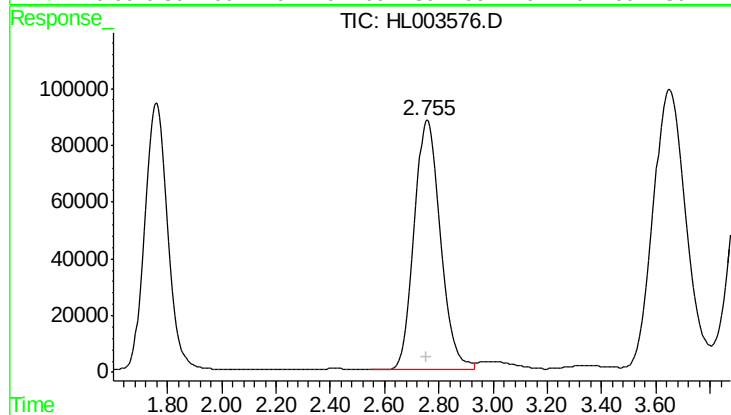

#4 1,3,5-Trinitrobenzene


R.T.: 2.757 min
Delta R.T.: 0.000 min
Response: 5889997
Conc: 485.16 ug/L

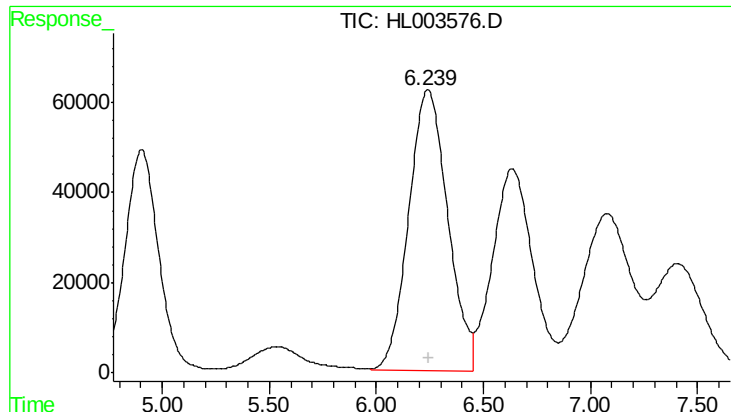

#5 Tetryl


R.T.: 6.241 min
Delta R.T.: -0.004 min
Response: 7898817
Conc: 925.47 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

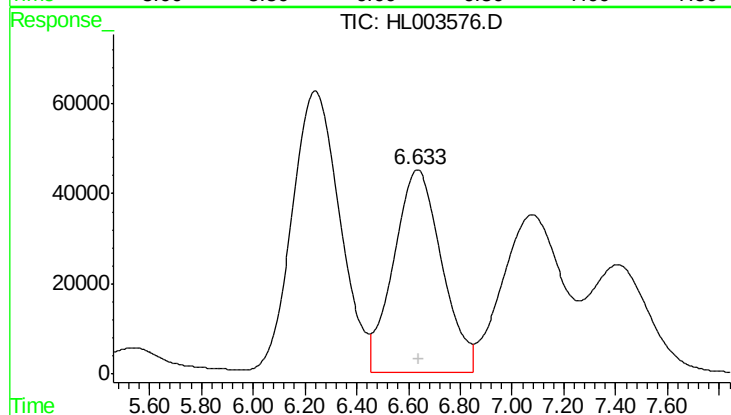


#6 2,4,6-Trinitrotoluene

R.T.: 6.635 min
Delta R.T.: -0.005 min
Response: 5812065
Conc: 515.80 ug/L

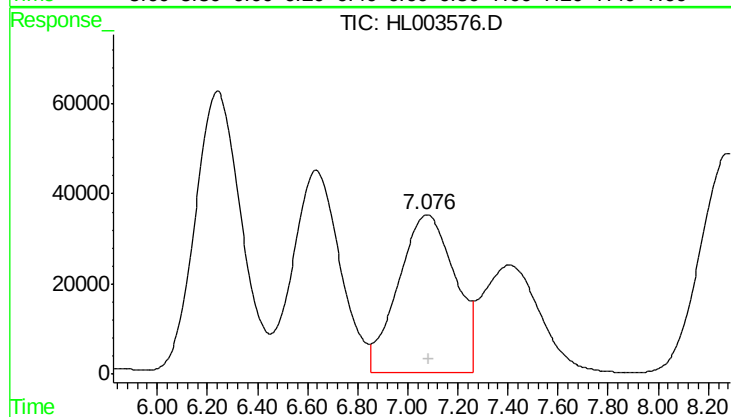


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.077 min
Delta R.T.: -0.007 min
Response: 5492666
Conc: 504.58 ug/L

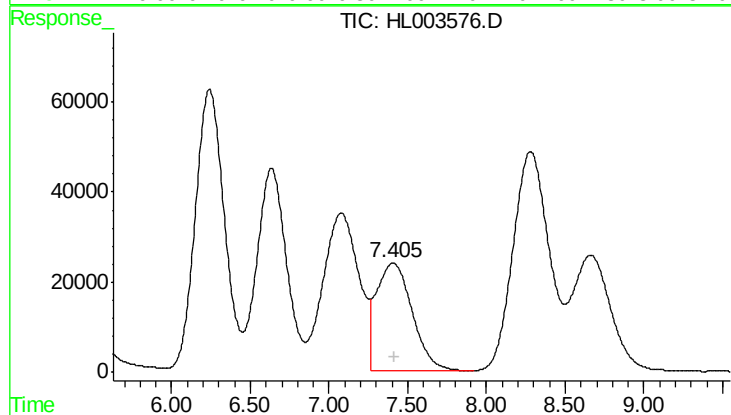

#8 4-Amino-2,6-dinitrotoluene


R.T.: 7.408 min
Delta R.T.: -0.008 min
Response: 3808940
Conc: 551.18 ug/L

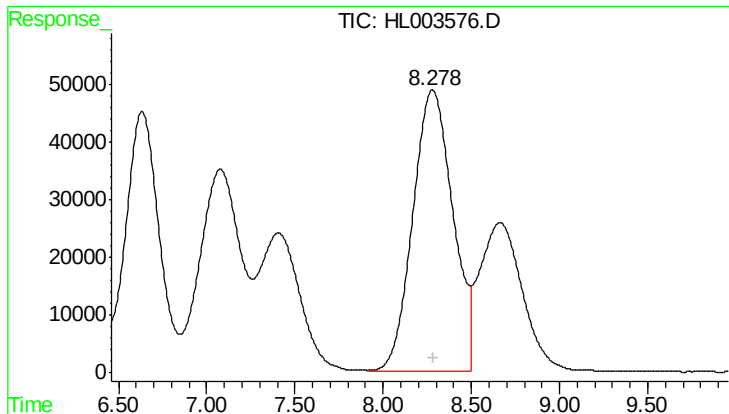

#9 2,4-Dinitrotoluene


R.T.: 8.280 min
Delta R.T.: -0.007 min
Response: 7709974
Conc: 510.79 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

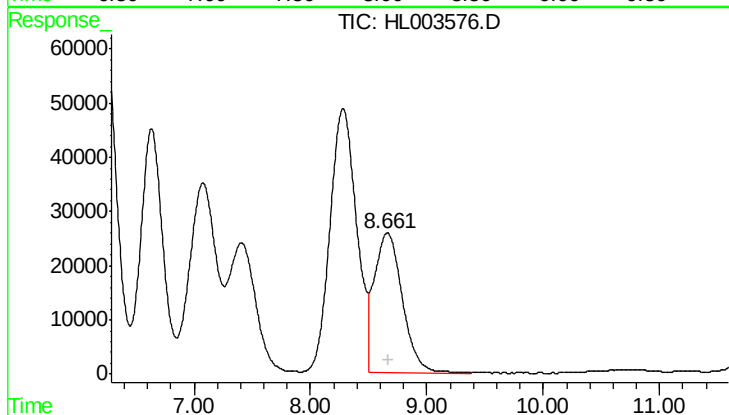


#10 2,6-Dinitrotoluene

R.T.: 8.663 min
Delta R.T.: -0.008 min
Response: 4355972
Conc: 500.45 ug/L

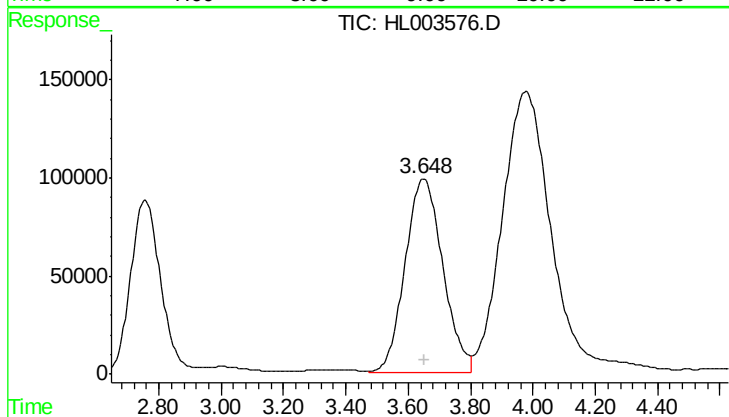


#11 1,3-Dinitrobenzene

R.T.: 3.650 min
Delta R.T.: -0.002 min
Response: 8317416
Conc: 525.00 ug/L

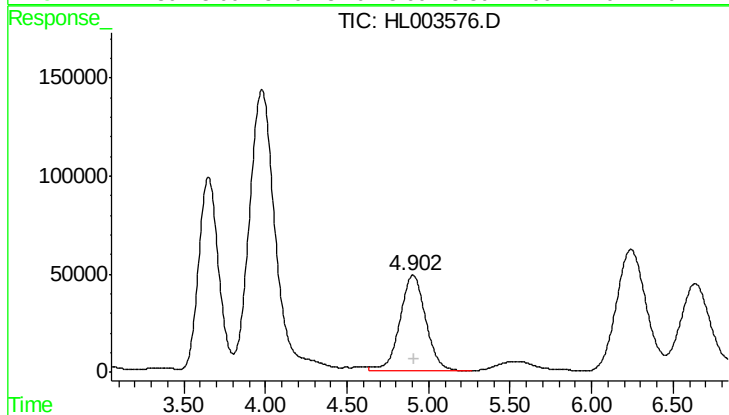

#12 Nitrobenzene


R.T.: 4.904 min
Delta R.T.: -0.004 min
Response: 5447845
Conc: 529.87 ug/L

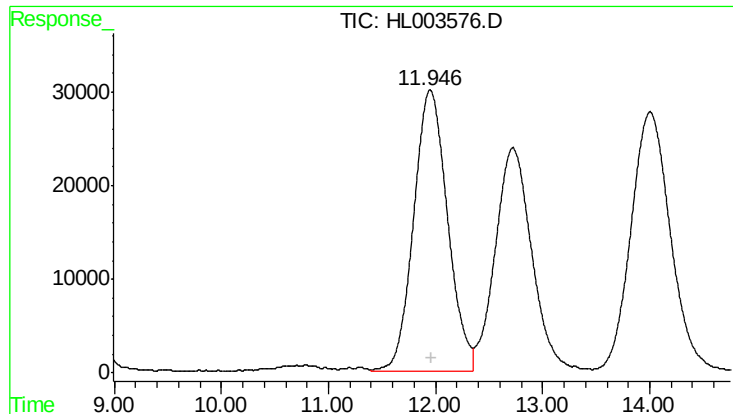

#13 2-Nitrotoluene


R.T.: 11.949 min
Delta R.T.: -0.014 min
Response: 6602302
Conc: 1001.16 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

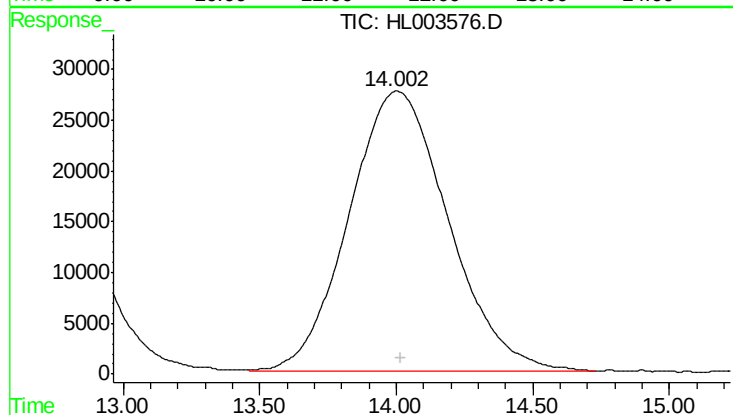


#14 3-Nitrotoluene

R.T.: 14.003 min
Delta R.T.: -0.012 min
Response: 6986359
Conc: 987.86 ug/L

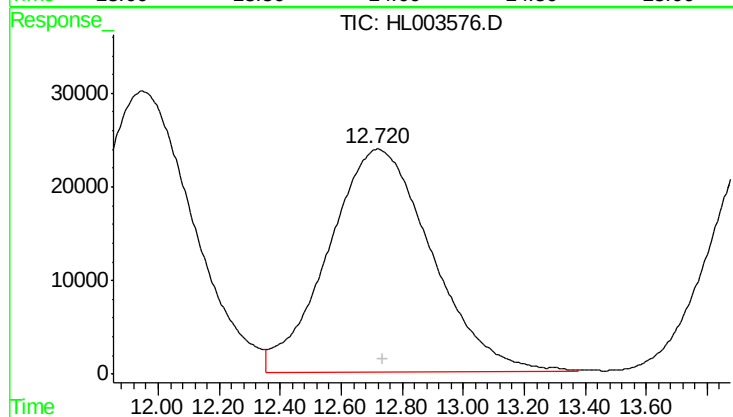


#15 4-Nitrotoluene

R.T.: 12.722 min
Delta R.T.: -0.014 min
Response: 5613876
Conc: 1017.04 ug/L

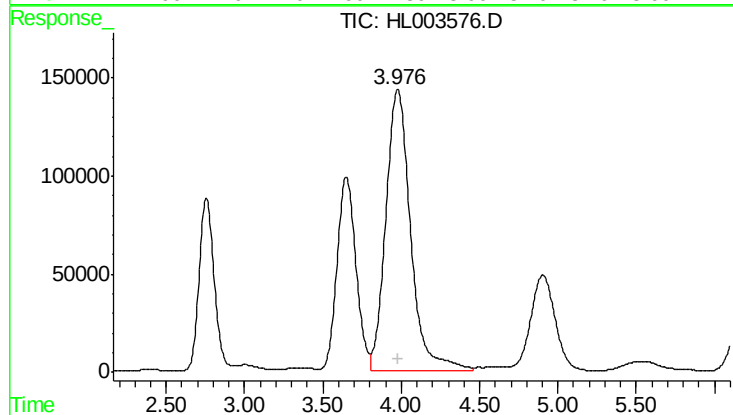

#16 3,5-Dinitroaniline

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 15896938
Conc: 1039.42 ug/L

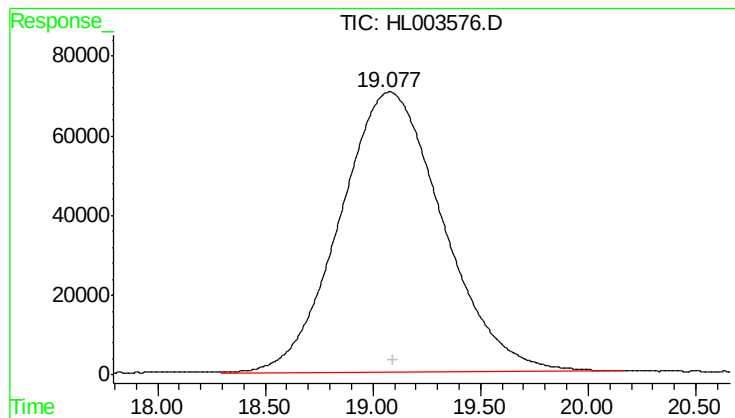

#18 PETN

R.T.: 19.078 min
Delta R.T.: -0.016 min
Response: 23505184
Conc: 2429.46 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV