

Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL092916\  
Data File : HL006410.D  
Signal(s) : vwd1A.ch  
Acq On : 29-Sep-2016, 14:44  
Operator : UM/MA  
Sample : HSTDICC001  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
HSTDICC001

Manual Integrations  
APPROVED

umangi  
10/4/2016 7:07:46 PM

Integration File: AUTOINT1.E  
Quant Time: Sep 29 16:56:38 2016  
Quant Method : Z:\HPCHEM1\HPLC\_L\Methods\HL092816NG.M  
Quant Title :  
QLast Update : Thu Sep 29 16:56:29 2016  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T.  | Response | Conc Units   |
|-----------------------------|-------|----------|--------------|
| -----                       |       |          |              |
| System Monitoring Compounds |       |          |              |
| 1) S 4-Nitroaniline         | 2.183 | 1935692  | 0.372 ng/ulm |
|                             |       |          |              |
| Target Compounds            |       |          |              |
| 2) T Nitroglycerin          | 6.706 | 11429010 | 1.002 ng/ul  |
| -----                       |       |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL092916\  
Data File : HL006410.D  
Signal(s) : vwd1A.ch  
Acq On : 29-Sep-2016, 14:44  
Operator : UM/MA  
Sample : HSTDICC001  
Misc :  
ALS Vial : 12 Sample Multiplier: 1


Instrument :  
HPLC\_L  
ClientSampleId :  
HSTDICC001


Manual Integrations  
APPROVED

umangi  
10/4/2016 7:07:46 PM

Integration File: AUTOINT1.E  
Quant Time: Sep 29 16:56:38 2016  
Quant Method : Z:\HPCHEM1\HPLC\_L\Methods\HL092816NG.M  
Quant Title :  
QLast Update : Thu Sep 29 16:56:29 2016  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

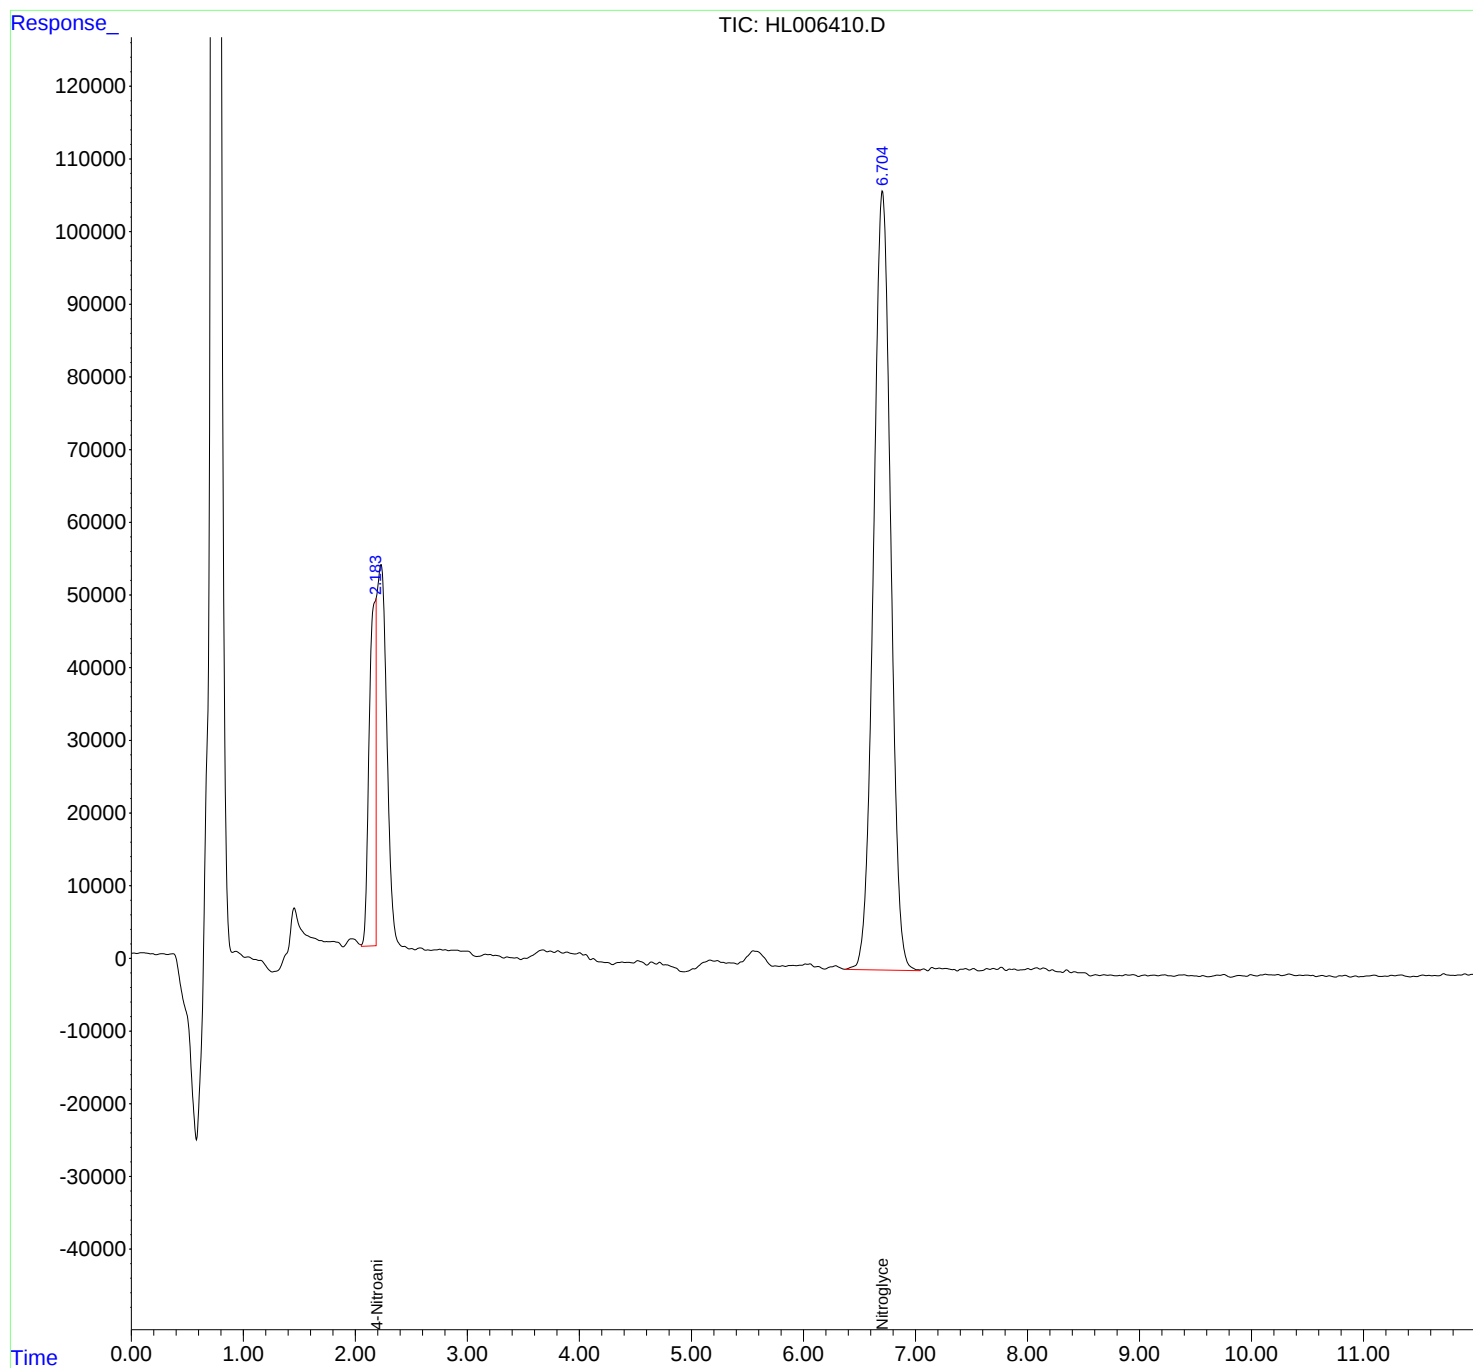

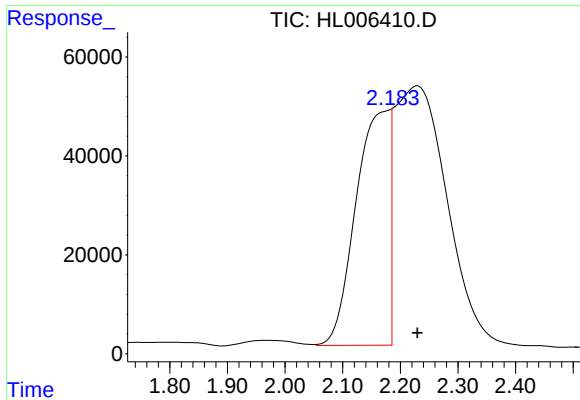


#1 4-Nitroaniline

R.T.: 2.183 min  
Delta R.T.: -0.047 min  
Response: 1935692  
Conc: 0.37 ng/ul m

Instrument :  
HPLC\_L  
ClientSampleId :  
HSTDICC001

Manual Integrations  
APPROVED

umangi  
10/4/2016 7:07:46 PM

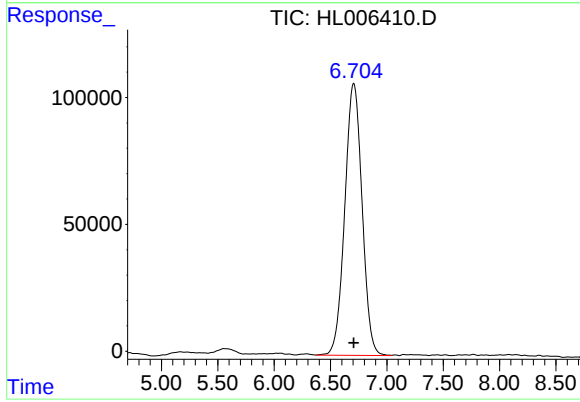

#2 Nitroglycerin

R.T.: 6.706 min  
Delta R.T.: 0.000 min  
Response: 11429010  
Conc: 1.00 ng/ul