

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005582.D Vial: 5
Acq On : 04-Oct-2013, 10:19 Operator: QM
Sample : HSTDICC0100 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Oct 7 15:51 2013 Quant Results File: HL100413.RES

Instrument :
HPLC_L
LabSampleId :
HSTDICC0100

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL100413.M
Title :
Last Update : Mon Oct 07 15:28:23 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
8) T Tetryl	6.36	1956550	320.467 ug/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005582.D HL100413.M Mon Oct 07 15:51:09 2013 RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005582.D Vial: 5
Acq On : 04-Oct-2013, 10:19 Operator: QM
Sample : HSTDICC0100 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Oct 7 15:51 2013 Quant Results File: HL100413.RES

Instrument :
HPLC_L
LabSampleId :
HSTDICC0100

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL100413.M
Title :
Last Update : Mon Oct 07 15:28:23 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

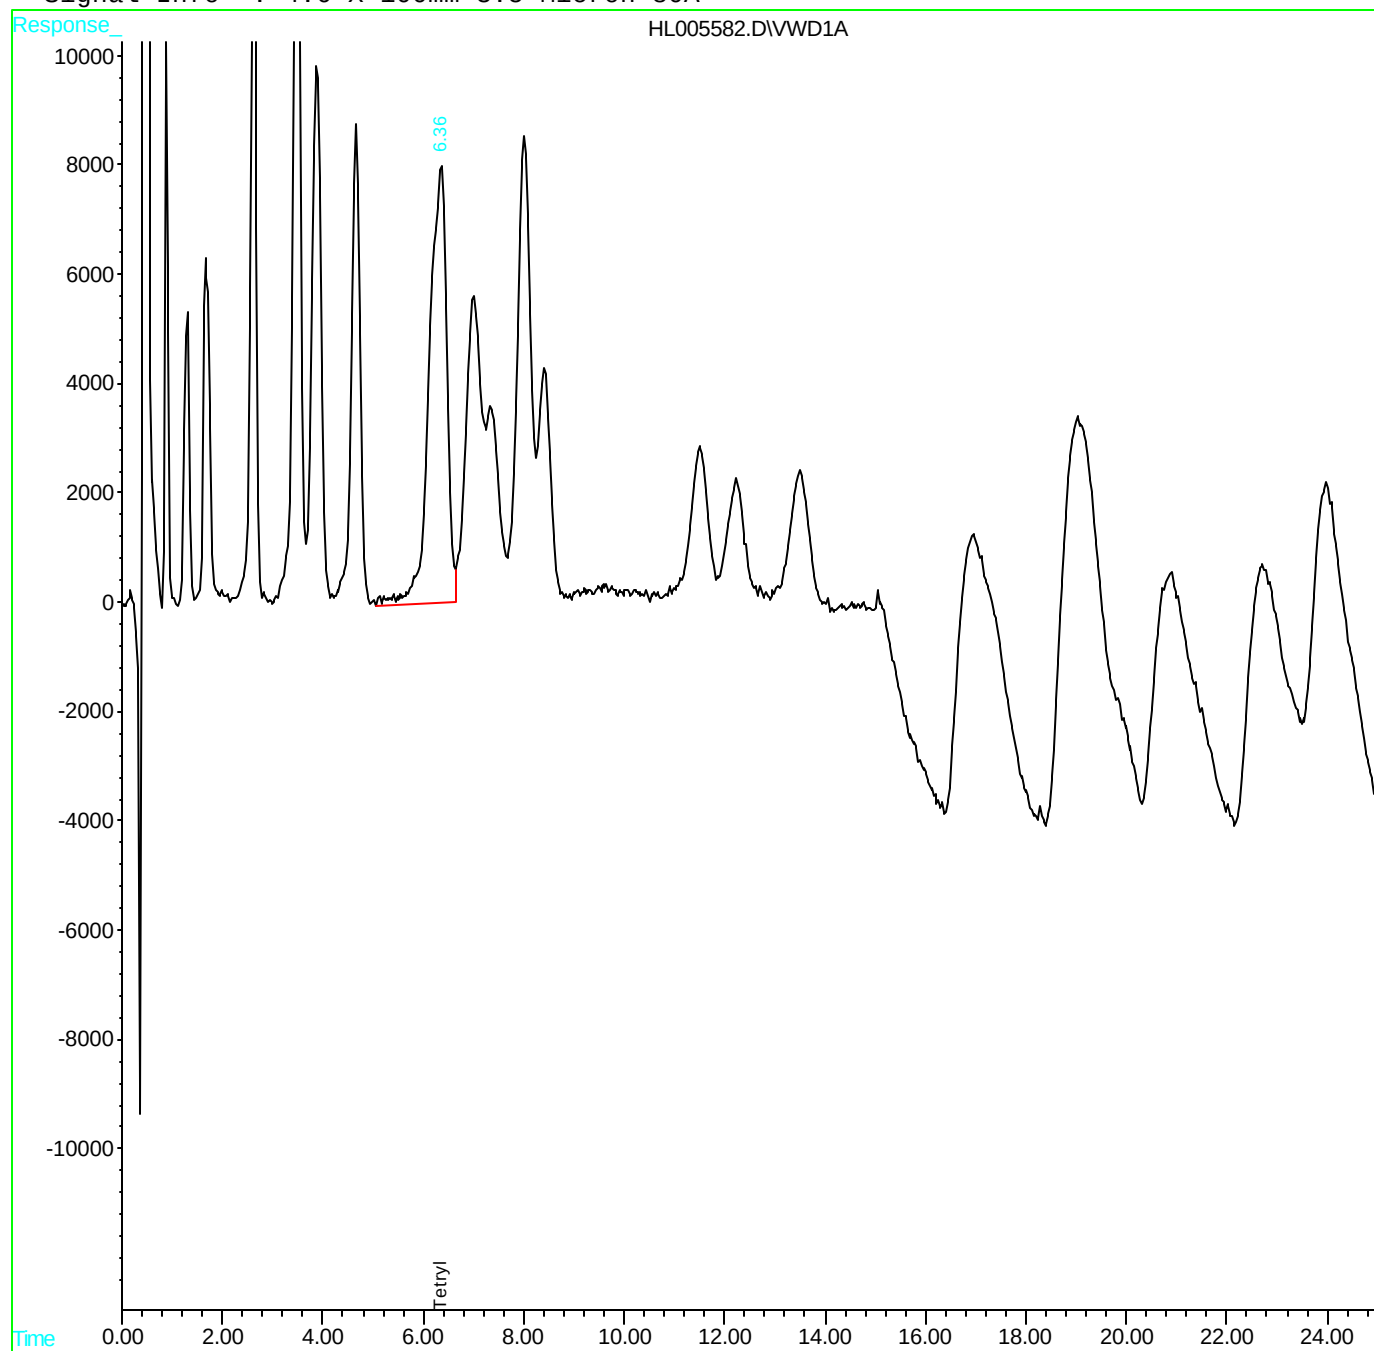


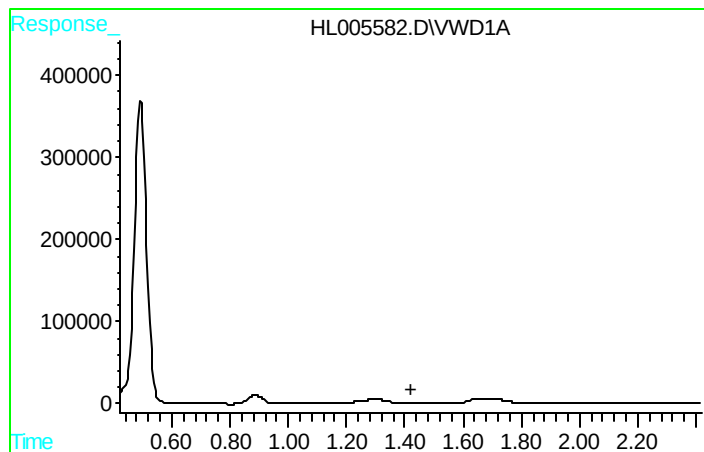

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 1.421 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
LabSampleId :
HSTDIC0100

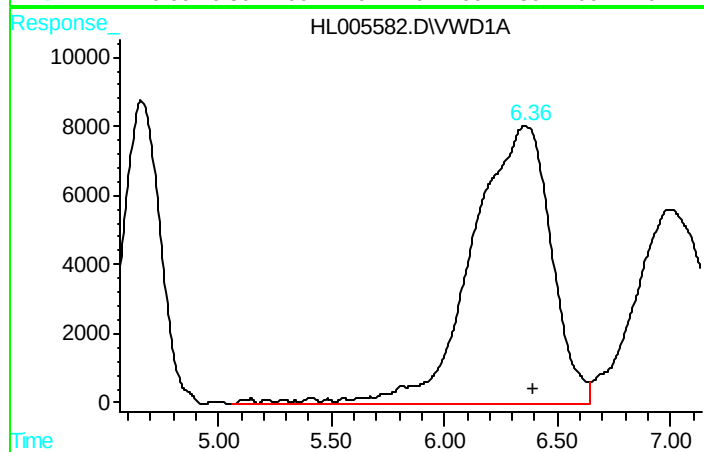

#8 Tetryl

R.T.: 6.359 min
Delta R.T.: -0.034 min
Response: 1956550
Conc: 320.47 ug/L