

Data File : Z:\HPCHEM1\HPLC\_L\DATA\HL100413\HL005584.D Vial: 7  
Acq On : 04-Oct-2013, 11:13 Operator: QM  
Sample : HSTDICV0500 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: Oct 7 18:33 2013 Quant Results File: HL100413.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
ICVHL100413

Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL100413.M  
Title :  
Last Update : Mon Oct 07 18:32:16 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

Target Compounds

|             |      |          |               |
|-------------|------|----------|---------------|
| 8) T Tetryl | 6.42 | 10239903 | 1741.804 ug/L |
|-------------|------|----------|---------------|

-----  
Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005584.D HL100413.M

Mon Oct 07 18:33:27 2013

RPT1


# Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_L\DATA\HL100413\HL005584.D Vial: 7  
Acq On : 04-Oct-2013, 11:13 Operator: QM  
Sample : HSTDICV0500 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: Oct 7 18:33 2013 Quant Results File: HL100413.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
ICVHL100413

Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL100413.M  
Title :  
Last Update : Mon Oct 07 18:32:16 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

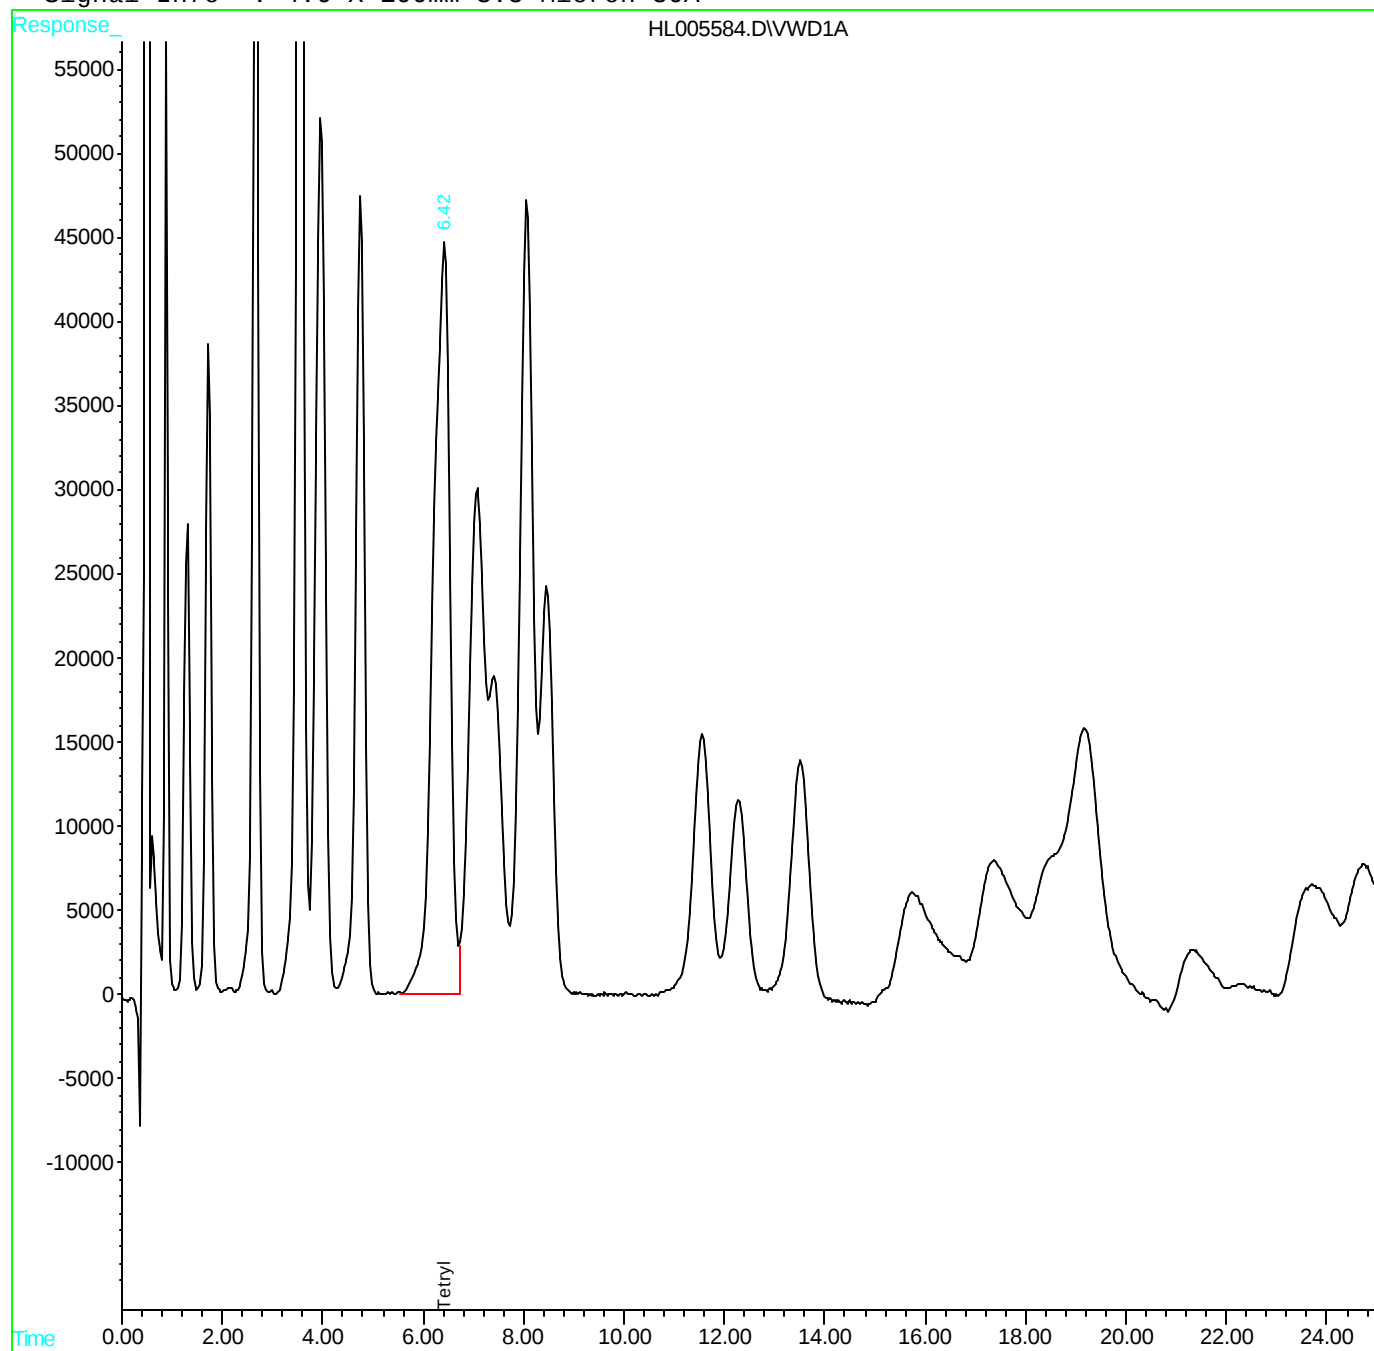


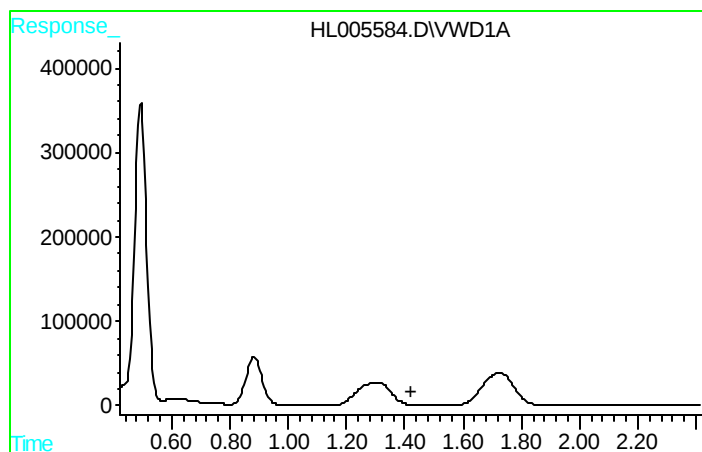

#1 4-Nitroaniline

R.T.: 0.000 min  
Exp R.T.: 1.421 min  
Response: 0  
Conc: N.D.

Instrument :  
HPLC\_L  
ClientSampleId :  
ICVHL100413

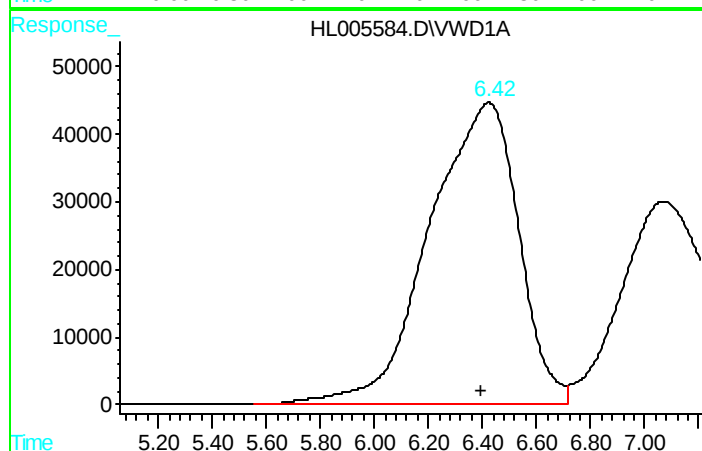

#8 Tetryl

R.T.: 6.423 min  
Delta R.T.: 0.031 min  
Response: 10239903  
Conc: 1741.80 ug/L