

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005585.D Vial: 8
Acq On : 04-Oct-2013, 12:01 Operator: QM
Sample : PB72592BS Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Oct 7 18:39 2013 Quant Results File: HL100413.RES

Instrument :
HPLC_L
ClientSampleId :
PB72592BS

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL100413.M
Title :
Last Update : Mon Oct 07 18:32:16 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) T HMX	0.90	879629	197.940 ug/L
8) T Tetryl	6.41	4222978	718.327 ug/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005585.D HL100413.M Mon Oct 07 18:39:25 2013 RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005585.D Vial: 8
Acq On : 04-Oct-2013, 12:01 Operator: QM
Sample : PB72592BS Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Oct 7 18:39 2013 Quant Results File: HL100413.RES

Instrument :
HPLC_L
ClientSampleId :
PB72592BS

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL100413.M
Title :
Last Update : Mon Oct 07 18:32:16 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

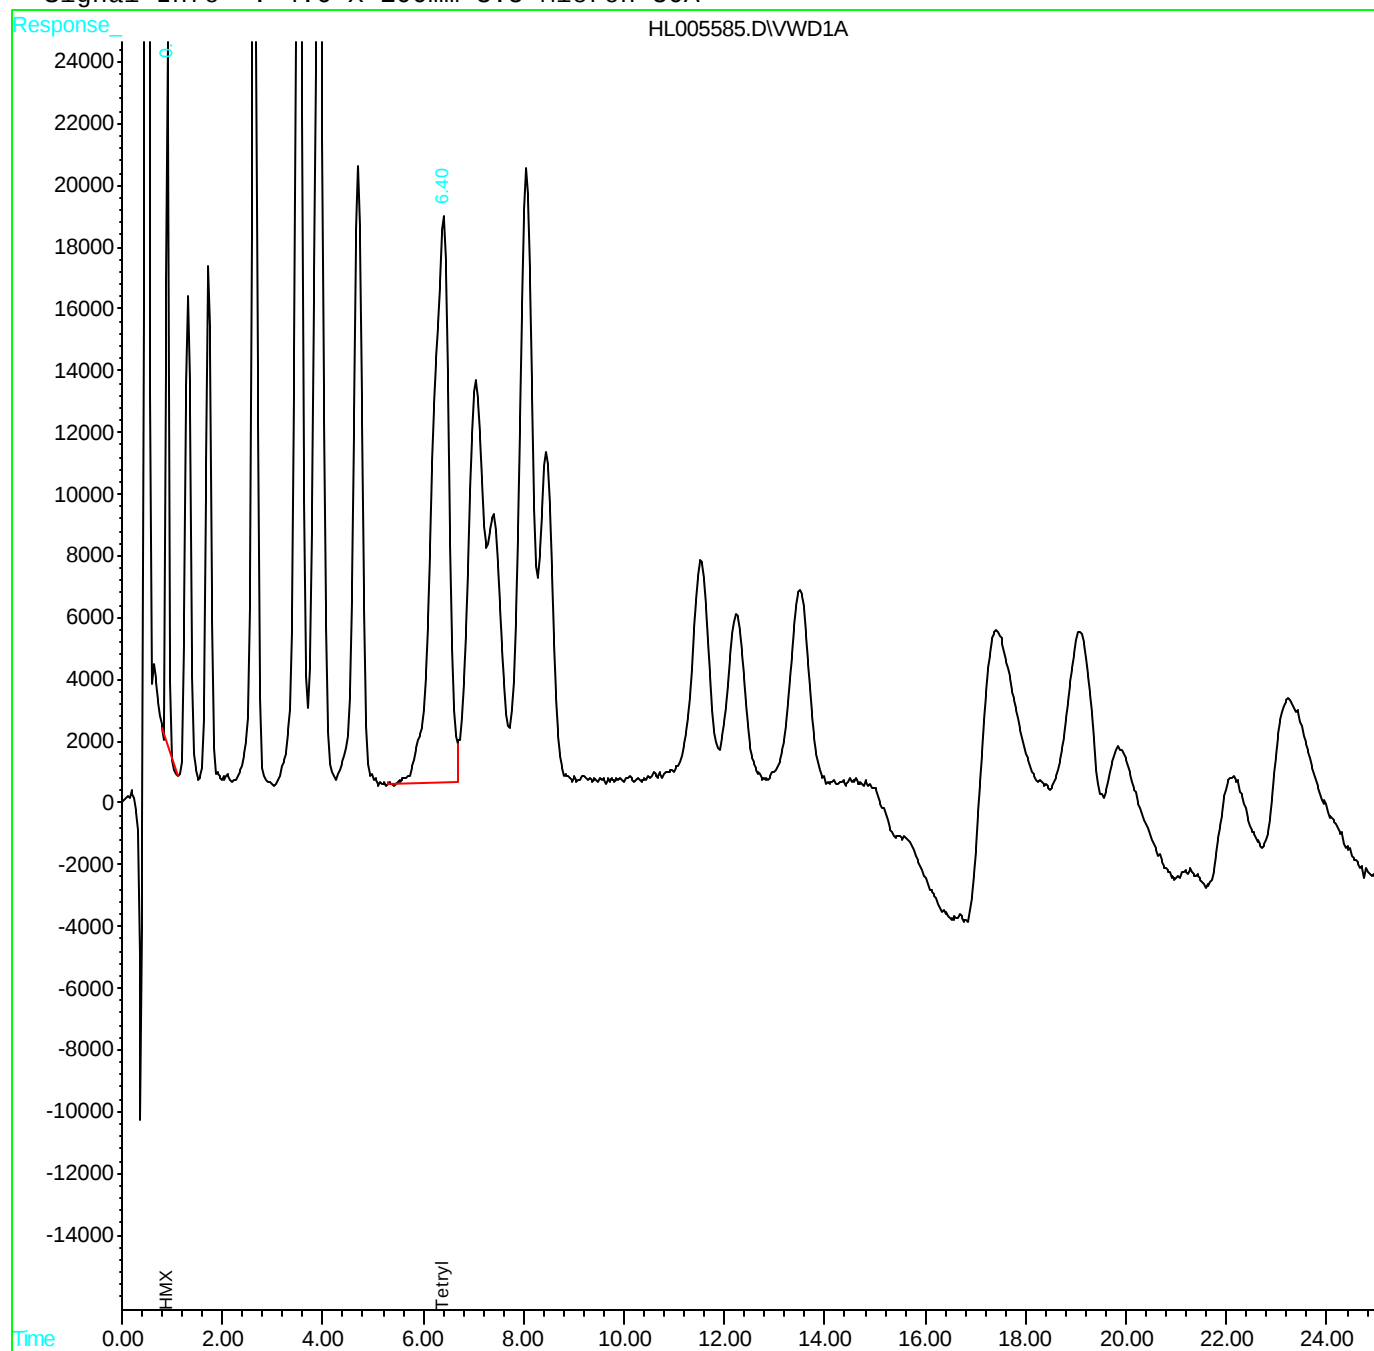


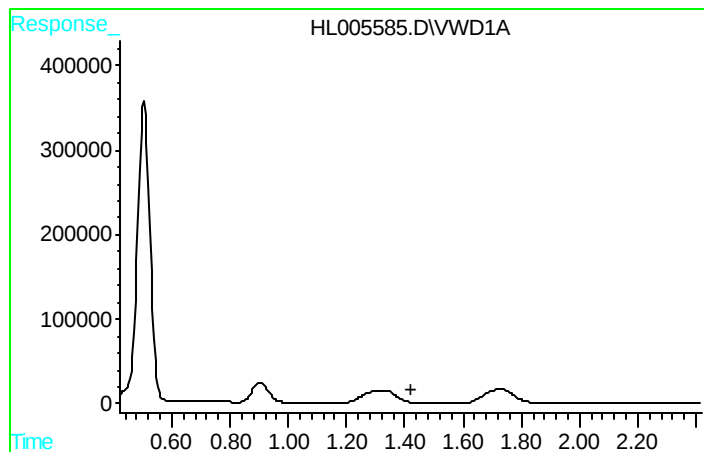

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 1.421 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
PB72592BS

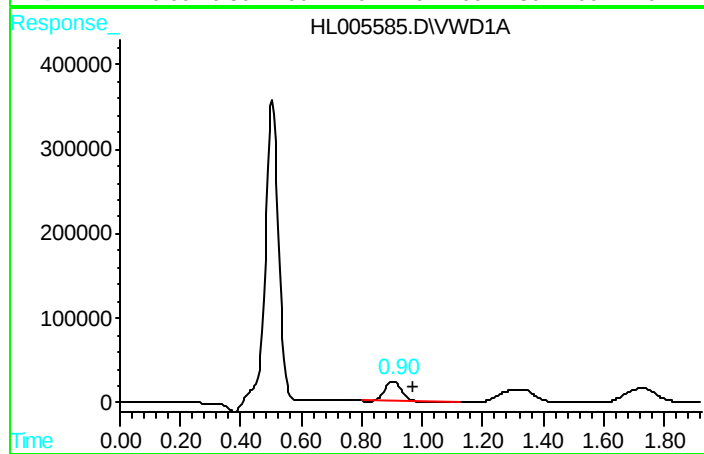

#2 HMX

R.T.: 0.904 min
Delta R.T.: -0.068 min
Response: 879629
Conc: 197.94 ug/L

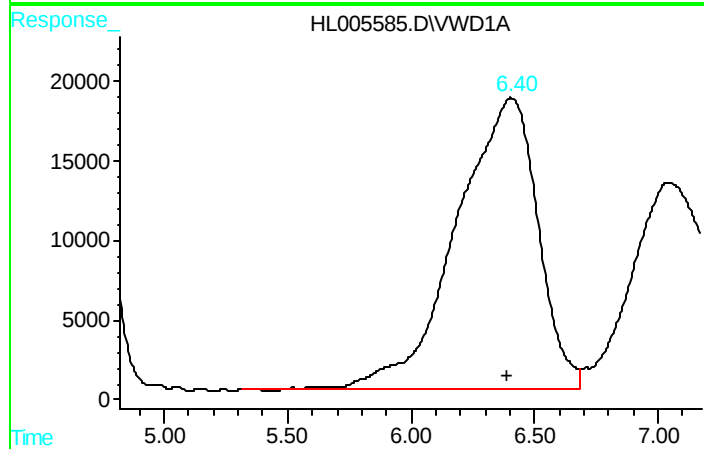

#8 Tetryl

R.T.: 6.406 min
Delta R.T.: 0.014 min
Response: 4222978
Conc: 718.33 ug/L