

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005588.D Vial: 4
Acq On : 04-Oct-2013, 13:22 Operator: QM
Sample : HSTDCCC0500 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Oct 7 18:48 2013 Quant Results File: HL100413.RES

Instrument :
HPLC_L
LabSampleId :
HSTDCCC0500

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL100413.M
Title :
Last Update : Mon Oct 07 18:32:16 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

8) T Tetryl	6.39	12287943	2090.175 ug/L
-------------	------	----------	---------------

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005588.D HL100413.M

Mon Oct 07 18:48:05 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005588.D Vial: 4
Acq On : 04-Oct-2013, 13:22 Operator: QM
Sample : HSTDCCC0500 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Oct 7 18:48 2013 Quant Results File: HL100413.RES

Instrument :
HPLC_L
LabSampleId :
HSTDCCC0500

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL100413.M
Title :
Last Update : Mon Oct 07 18:32:16 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

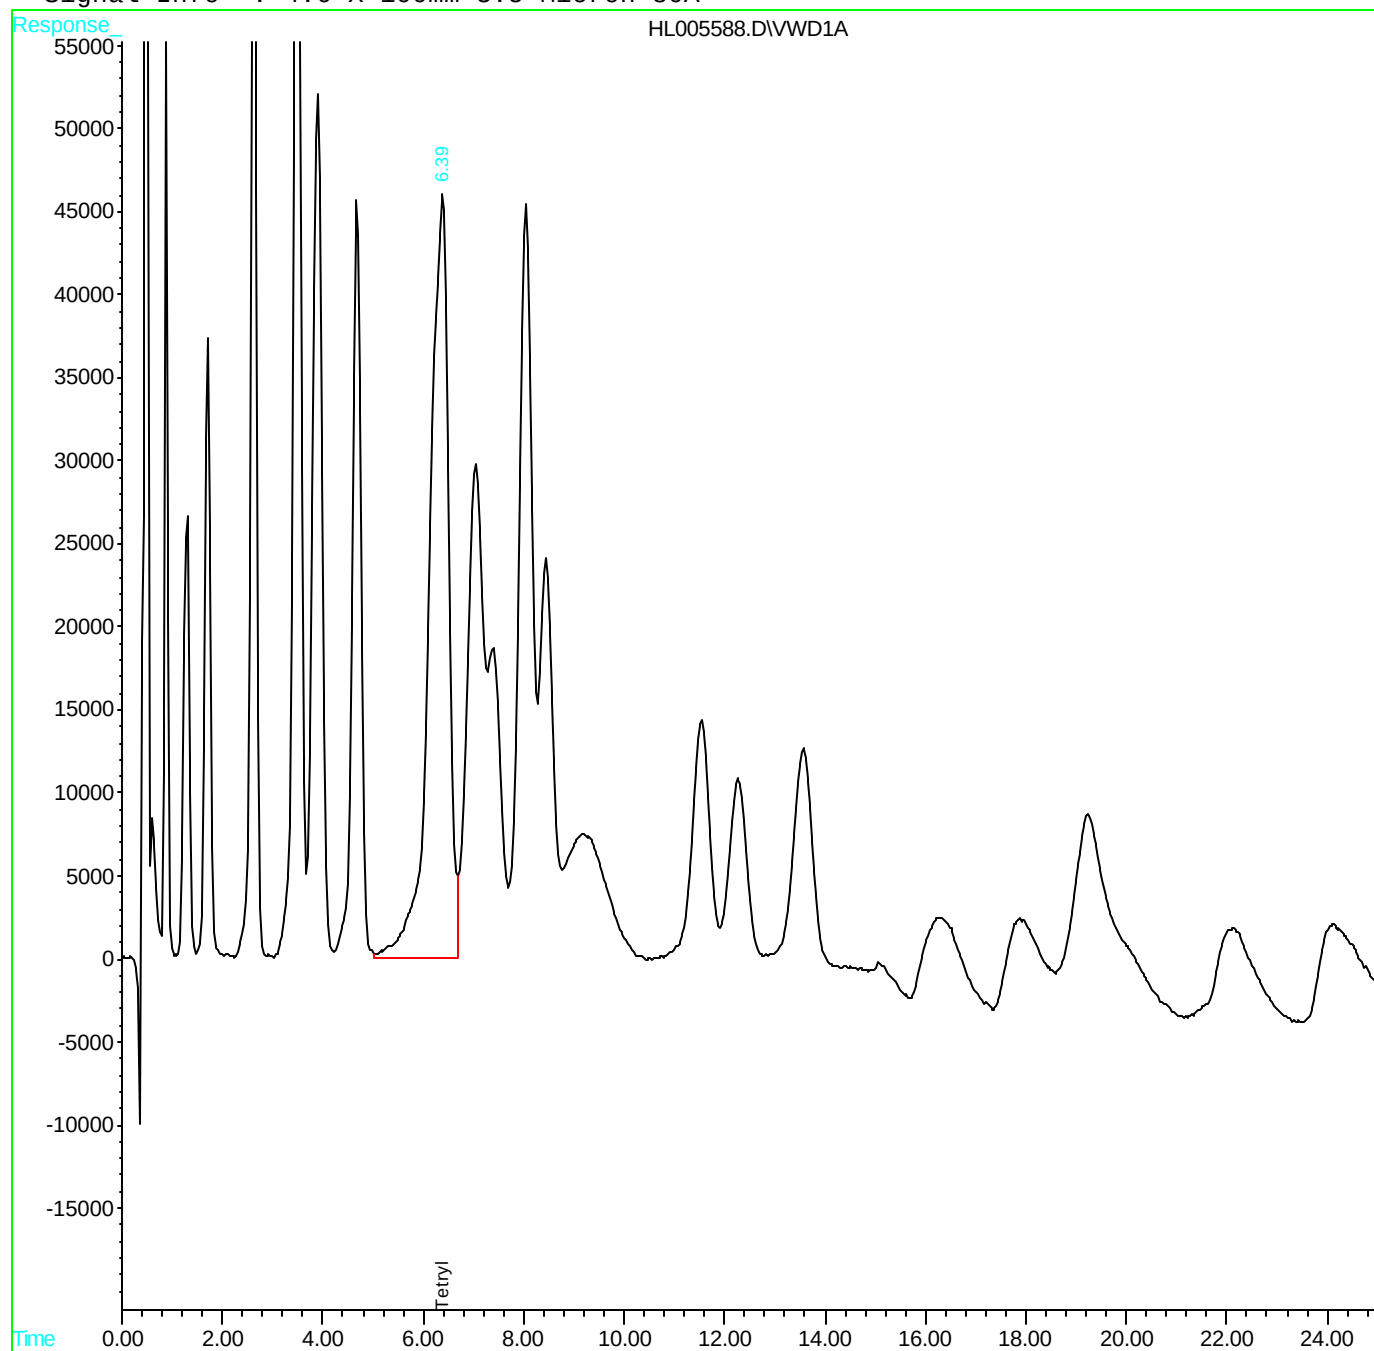


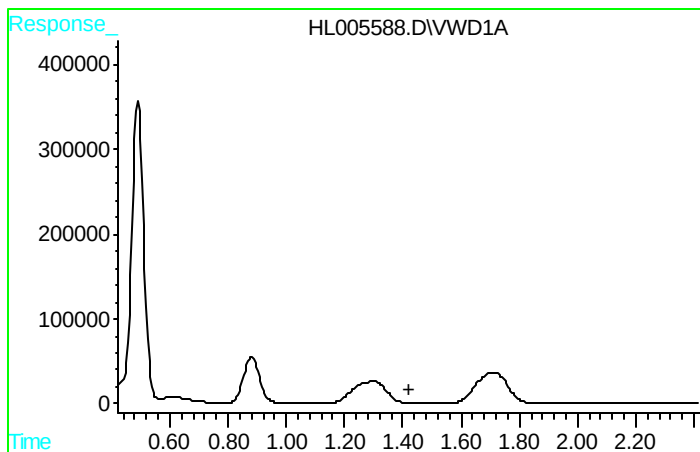

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 1.421 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
LabSampleId :
HSTDCCC0500

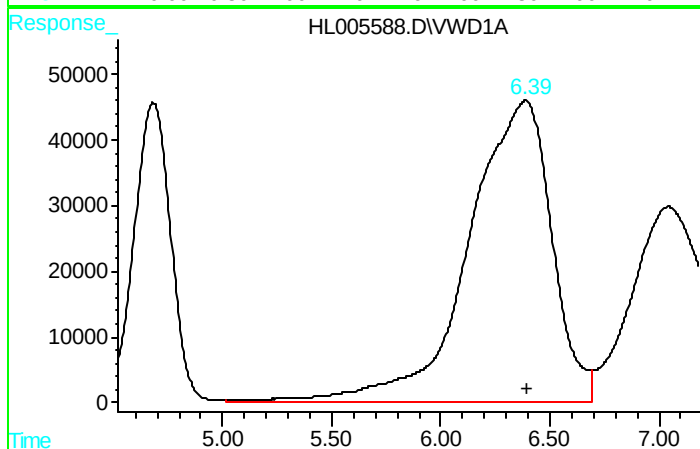

#8 Tetryl

R.T.: 6.388 min
Delta R.T.: -0.005 min
Response: 12287943
Conc: 2090.18 ug/L