

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005593.D Vial: 45
Acq On : 04-Oct-2013, 14:37 Operator: QM
Sample : HSTDICC001 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Oct 7 18:10 2013 Quant Results File: HL1004NG.RES

Instrument :
HPLC_L
LabSampleId :
HSTDICC001

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL1004NG.M
Title :
Last Update : Mon Oct 07 18:04:20 2013
Response via : Initial Calibration
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.29	4397971	1.067 ng/ul
Target Compounds			
2) T Nitroglycerin	6.05	7888791	0.864 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005593.D HL1004NG.M

Mon Oct 07 18:10:09 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005593.D Vial: 45
Acq On : 04-Oct-2013, 14:37 Operator: QM
Sample : HSTDICC001 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Oct 7 18:10 2013 Quant Results File: HL1004NG.RES

Instrument :
HPLC_L
LabSampleId :
HSTDICC001

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL1004NG.M
Title :
Last Update : Mon Oct 07 18:04:20 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

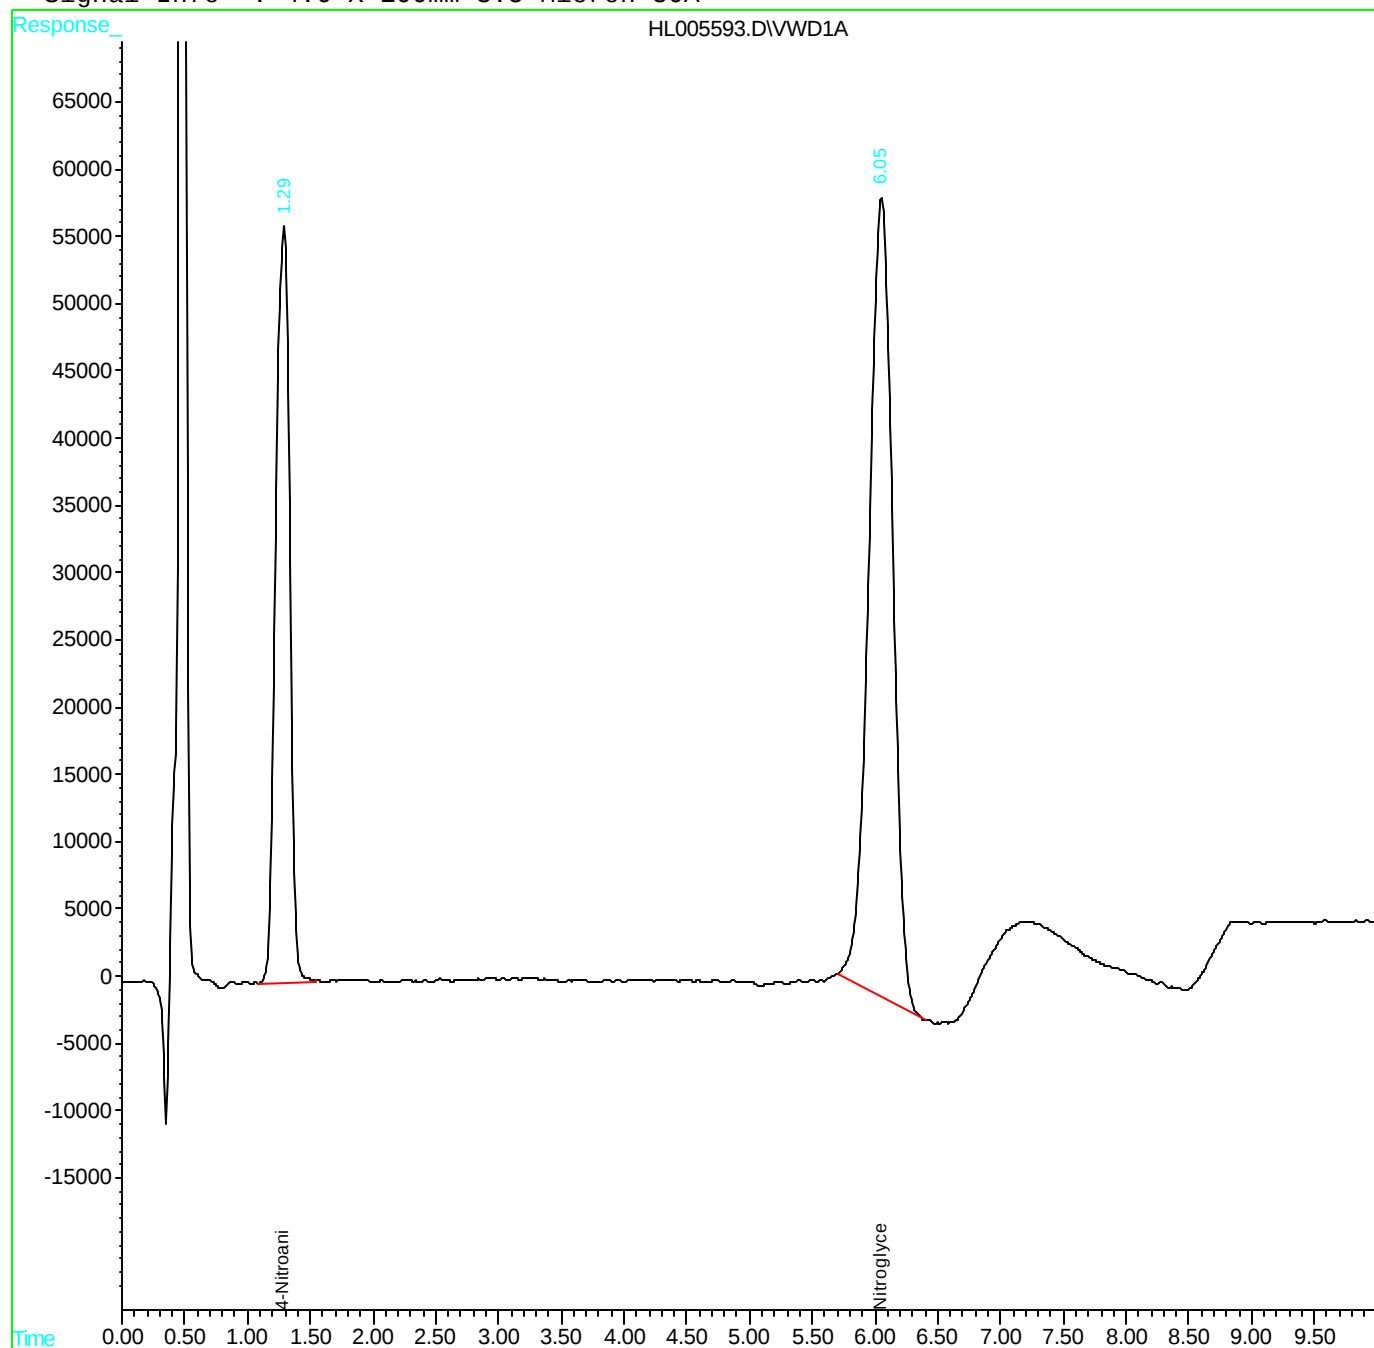


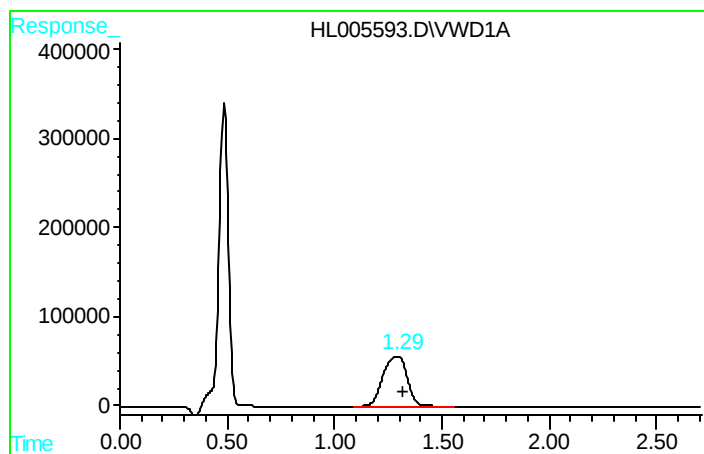

#1 4-Nitroaniline

R.T.: 1.294 min
Delta R.T.: -0.026 min
Response: 4397971
Conc: 1.07 ng/ul

Instrument :
HPLC_L
LabSampleId :
HSTDIC001

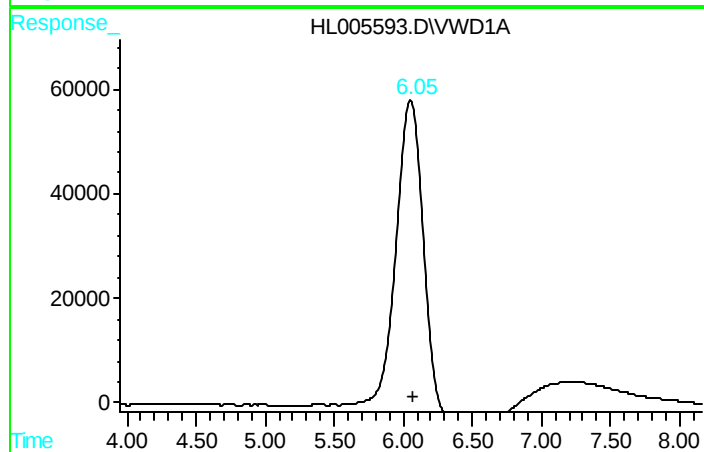

#2 Nitroglycerin

R.T.: 6.053 min
Delta R.T.: -0.017 min
Response: 7888791
Conc: 0.86 ng/ul