

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005586.D Vial: 9
Acq On : 04-Oct-2013, 12:28 Operator: QM
Sample : PB72592BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Oct 7 18:45 2013 Quant Results File: HL100413.RES

Instrument :
HPLC_L
ClientSampleId :
PB72592BL

Manual Integrations
APPROVED

mohammad
10/9/2013 3:41:56 PM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL100413.M
Title :
Last Update : Mon Oct 07 18:32:16 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.32	1274452	277.189 ug/L m

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005586.D HL100413.M

Tue Oct 08 19:16:27 2013

RPT1

Quantitation Report

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005586.D Vial: 9
Acq On : 04-Oct-2013, 12:28 Operator: QM
Sample : PB72592BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Oct 7 18:45 2013 Quant Results File: HL100413.RES


Instrument :
HPLC_L
ClientSampleId :
PB72592BL


Manual Integrations
APPROVED

mohammad
10/9/2013 3:41:56 PM

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL100413.M
Title :
Last Update : Mon Oct 07 18:32:16 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

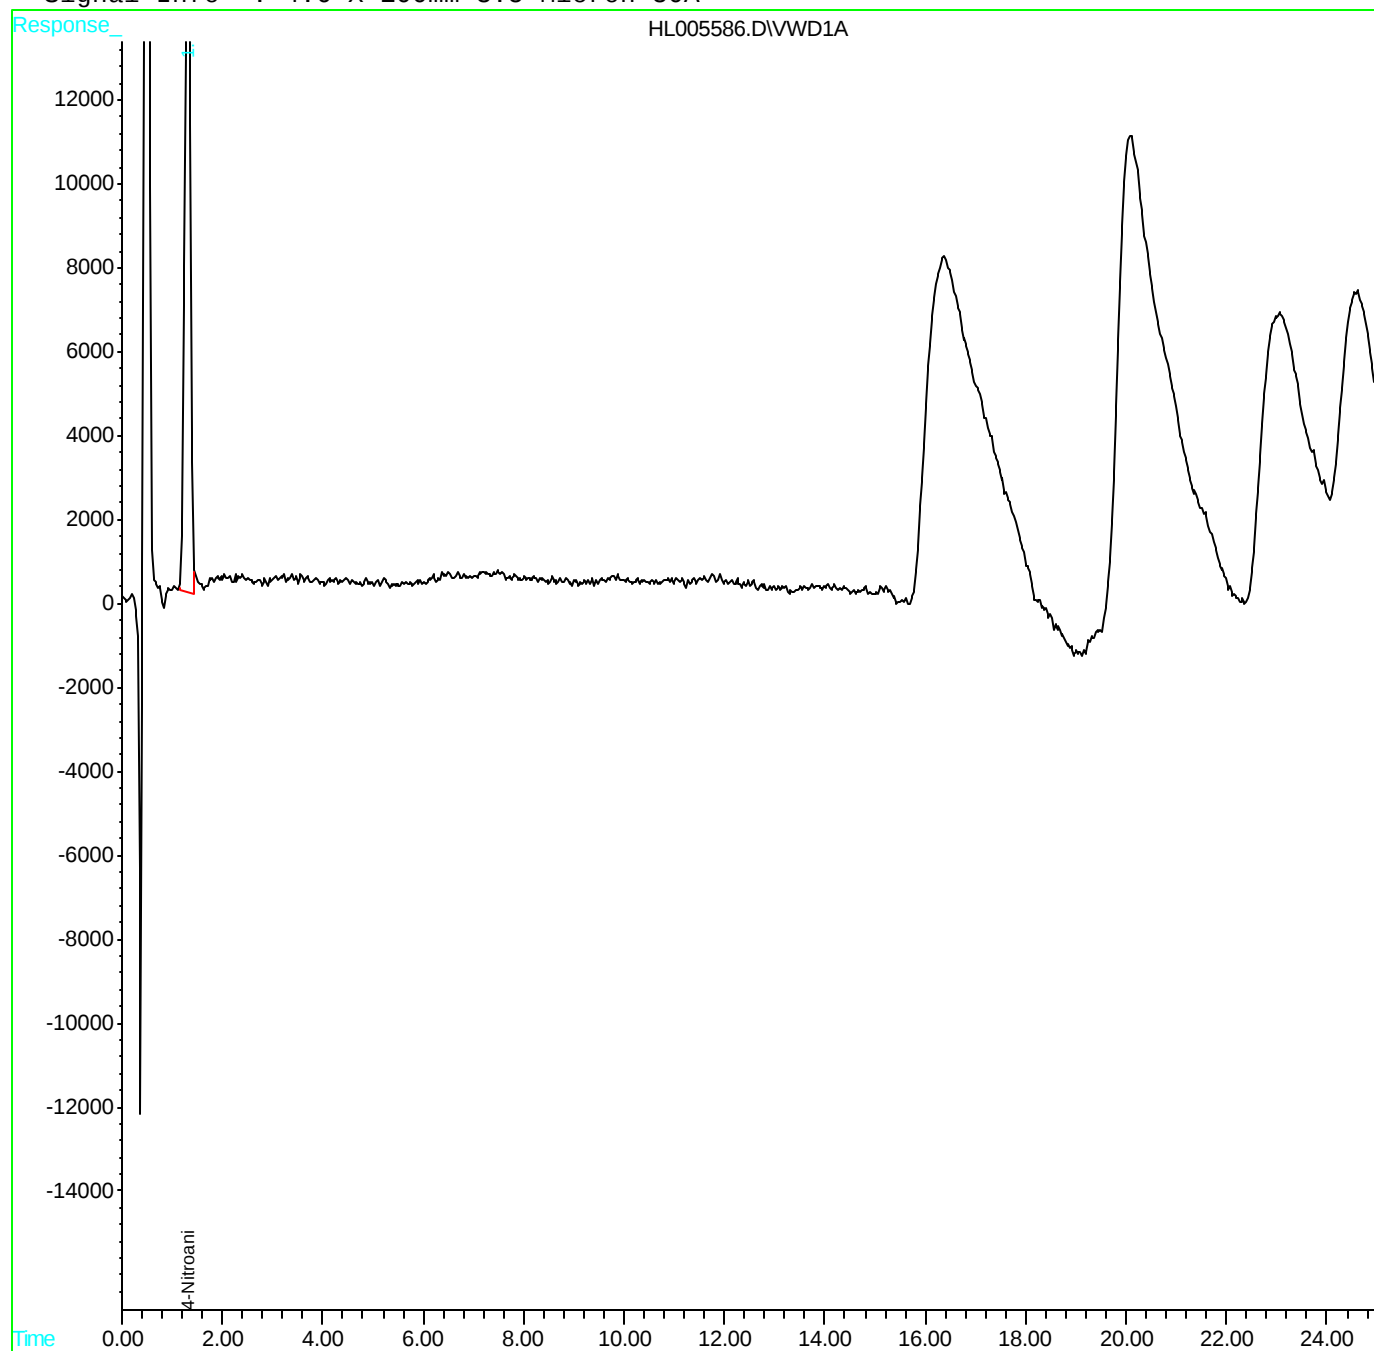

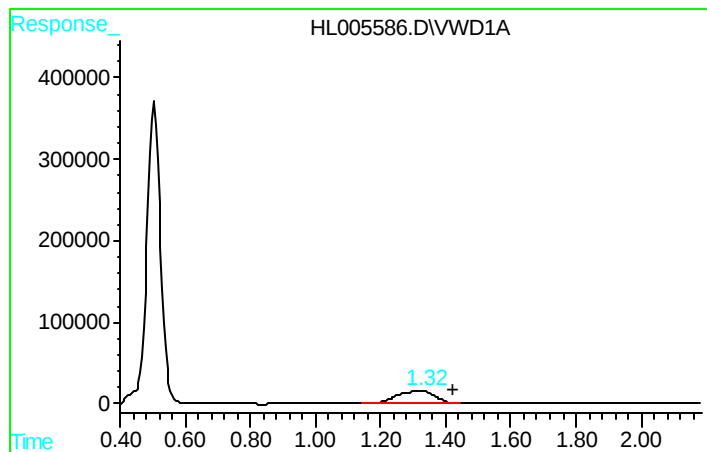

#1 4-Nitroaniline

R.T.: 1.322 min
Delta R.T.: -0.100 min
Response: 1274452
Conc: 277.19 ug/L m

Instrument :

HPLC_L

ClientSampleId :

PB72592BL

Manual Integrations
APPROVED

mohammad
10/9/2013 3:41:56 PM