

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005595.D Vial: 47
Acq On : 04-Oct-2013, 15:01 Operator: QM
Sample : HSTDICV005 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Oct 7 18:56 2013 Quant Results File: HL1004NG.RES

Instrument :
HPLC_L
ClientSampleId :
ICVHL100413NG

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL1004NG.M
Title :
Last Update : Mon Oct 07 18:04:20 2013
Response via : Initial Calibration
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.34	21217282	4.934 ng/ul
Target Compounds			
2) T Nitroglycerin	6.11	41232990	5.130 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005595.D HL1004NG.M

Tue Oct 08 19:20:43 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL100413\HL005595.D Vial: 47
Acq On : 04-Oct-2013, 15:01 Operator: QM
Sample : HSTDICV005 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Oct 7 18:56 2013 Quant Results File: HL1004NG.RES

Instrument :
HPLC_L
ClientSampleId :
ICVHL100413NG

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL1004NG.M
Title :
Last Update : Mon Oct 07 18:04:20 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

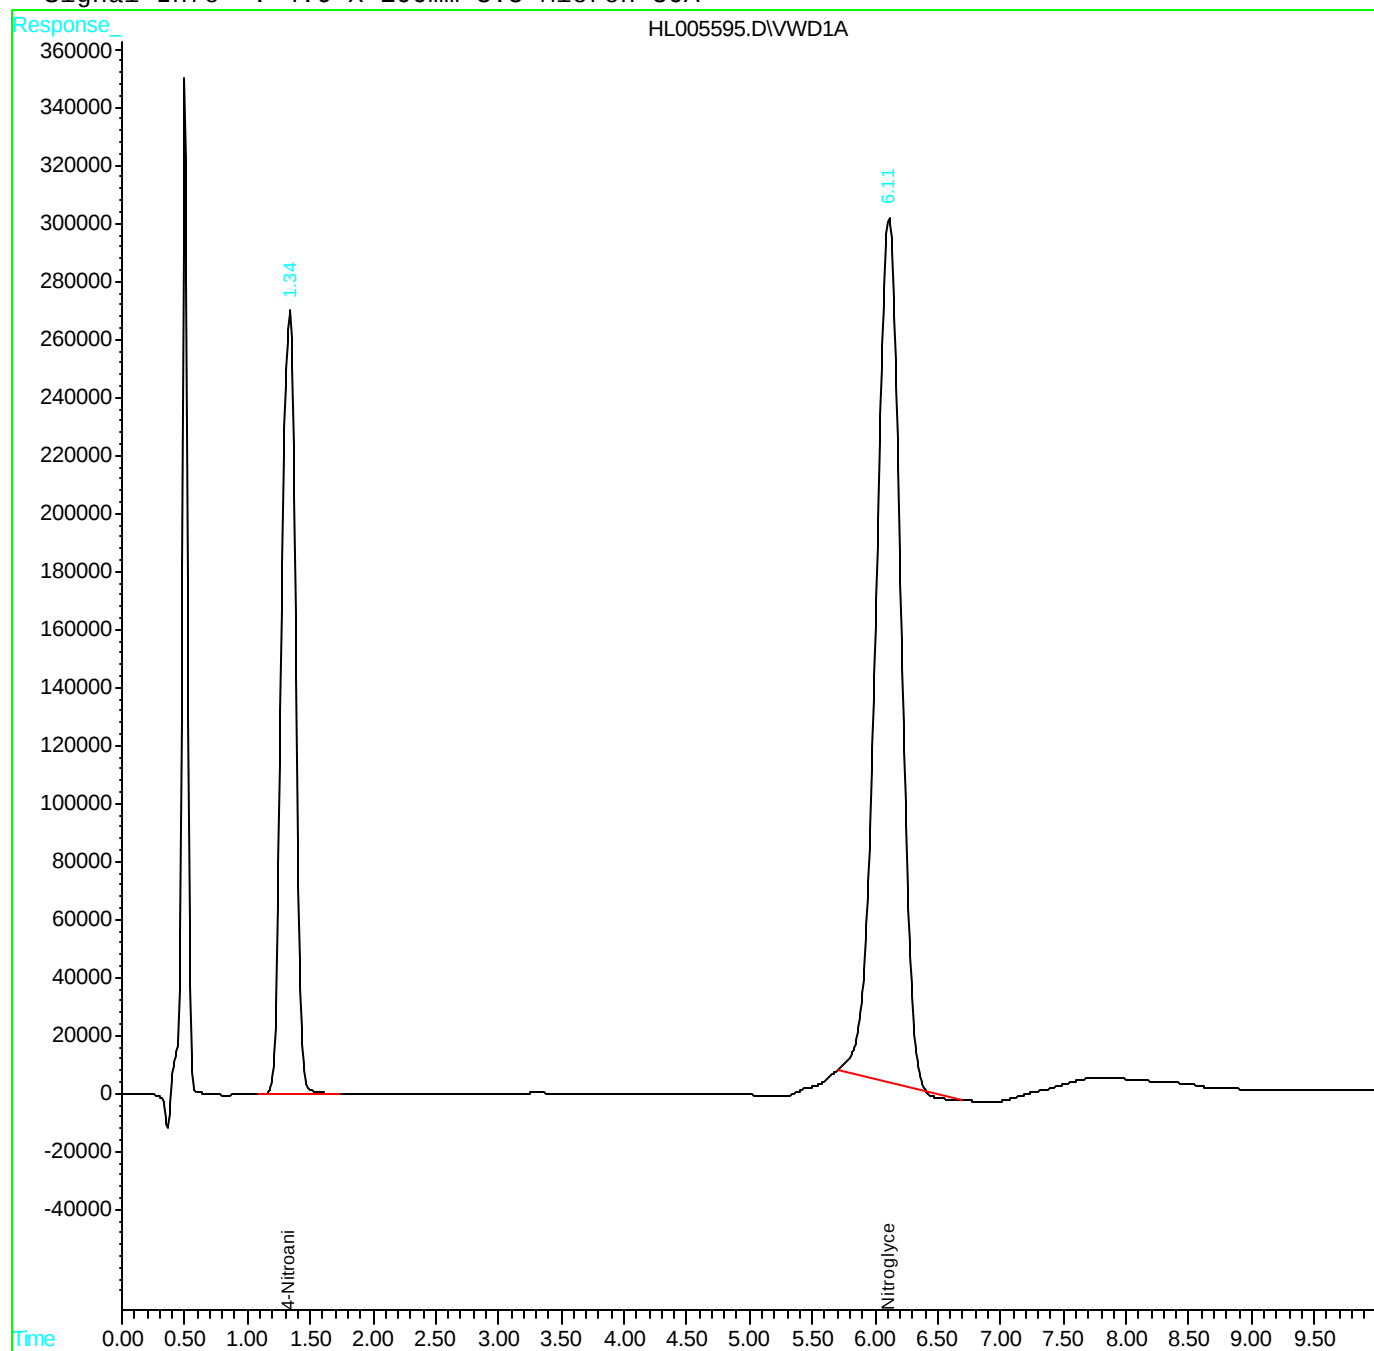


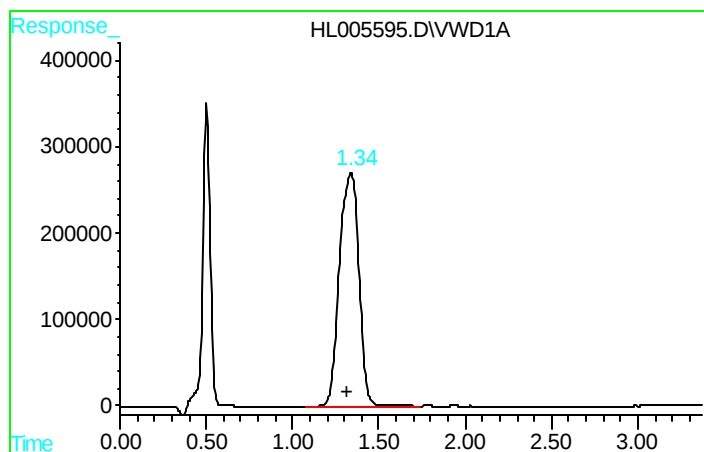

#1 4-Nitroaniline

R.T.: 1.341 min
Delta R.T.: 0.021 min
Response: 21217282
Conc: 4.93 ng/ul

Instrument :
HPLC_L
ClientSampleId :
ICVHL100413NG

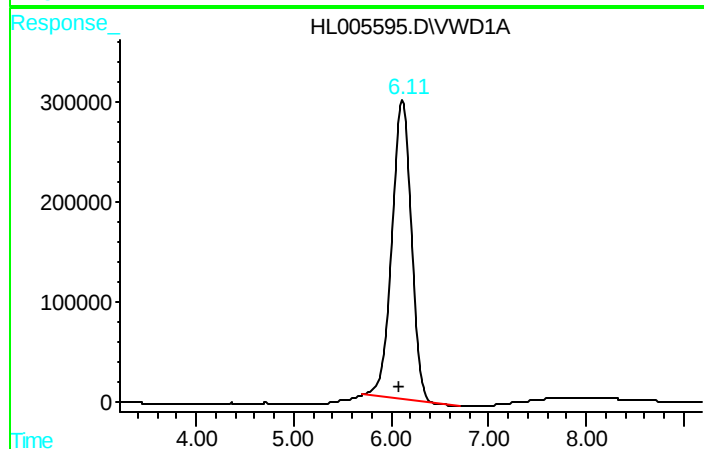

#2 Nitroglycerin

R.T.: 6.112 min
Delta R.T.: 0.042 min
Response: 41232990
Conc: 5.13 ng/ul