

Data Path : Z:\HPCHEM1\HPLC_L\HL102214\
 Data File : HL005662.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 22-Oct-2014, 19:08
 Operator : TP
 Sample : HSTDICC5000
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDICC5000

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 16:51:37 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
 Quant Title :
 QLast Update : Mon Mar 09 16:43:57 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.697f	19876555	1532.915 ug/L
Target Compounds			
3) T RDX	2.697f	19876555	1532.915 ug/L
5) T 1,3-Dinitrobenzene	5.753	121497366	5014.455 ng/ml
6) T 3,5-Dinitroaniline	6.592	87144253	5008.374 ug/L
7) T Nitrobenzene	7.377f	74040865	4996.696 ug/L
9) T 2,4,6-Trinitrotoluene	10.427	79362831	5434.994 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\HL102214\
Data File : HL005662.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 22-Oct-2014, 19:08
Operator : TP
Sample : HSTDICC5000
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICC5000

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:51:37 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Quant Title :
QLast Update : Mon Mar 09 16:43:57 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

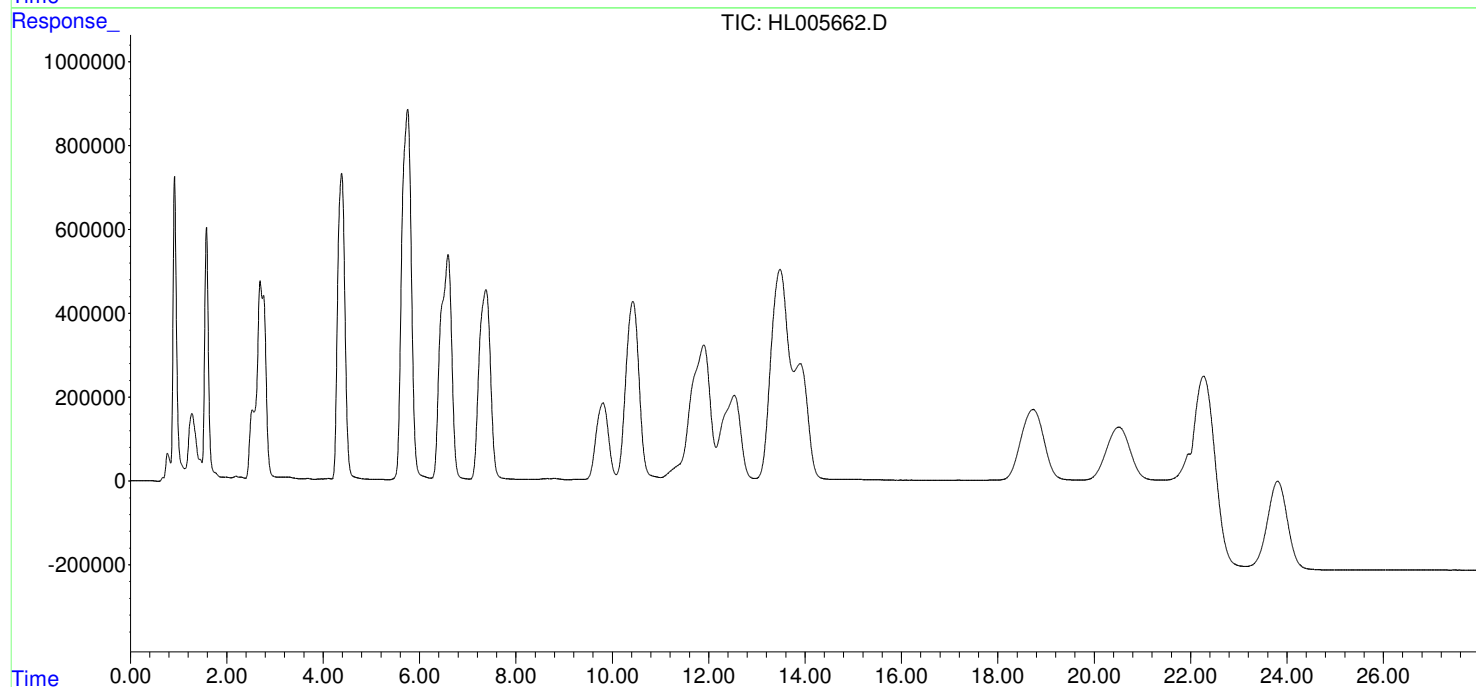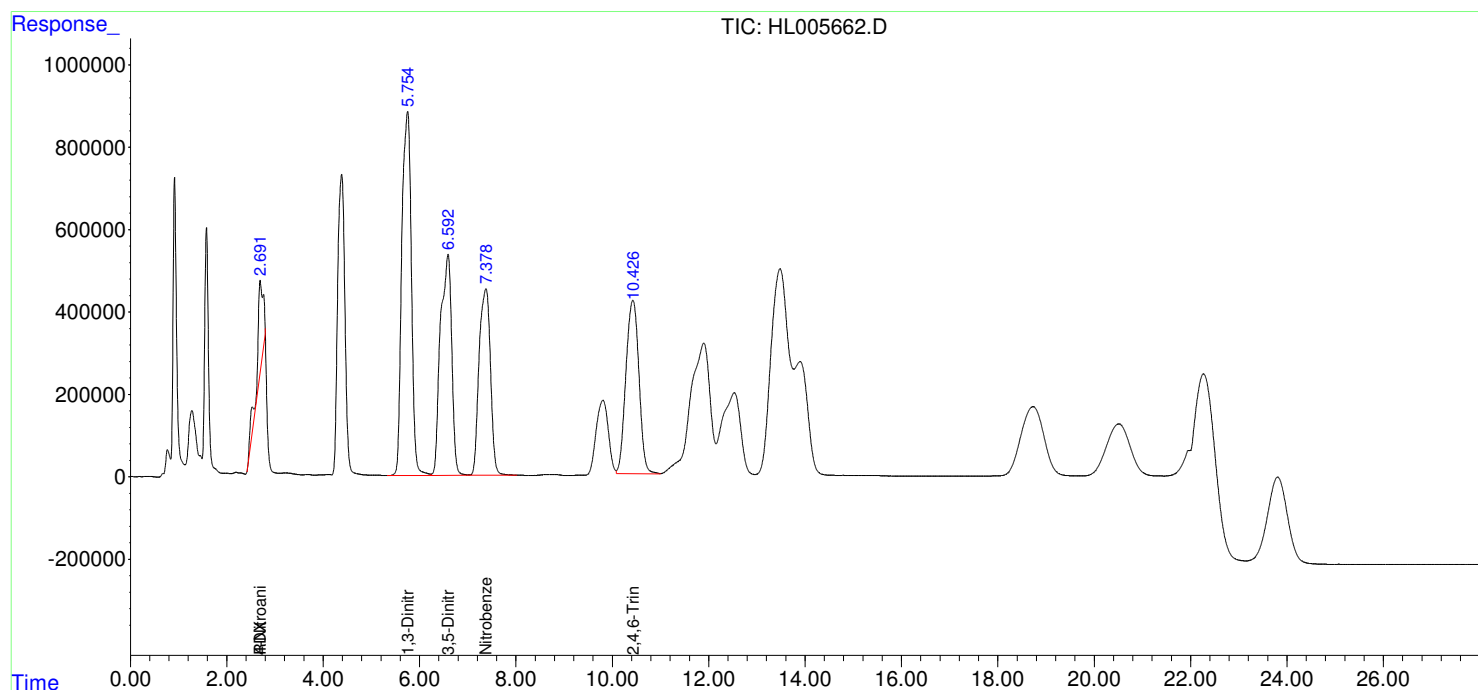


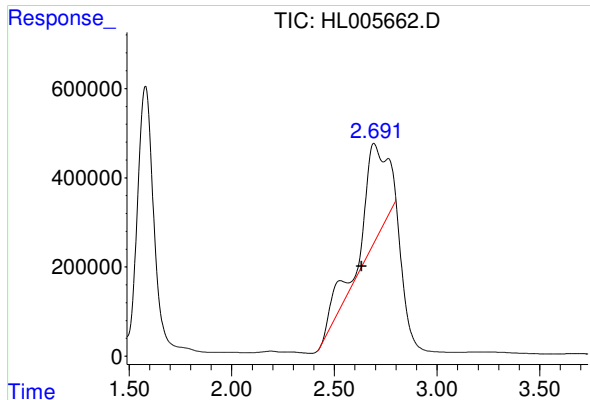

#1 4-Nitroaniline


R.T.: 2.697 min
Delta R.T.: 0.065 min
Response: 19876555
Conc: 1532.91 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC5000

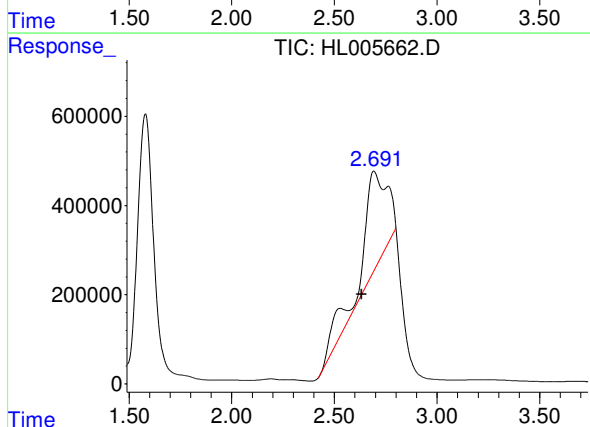


#3 RDX

R.T.: 2.697 min
Delta R.T.: 0.065 min
Response: 19876555
Conc: 1532.91 ug/L

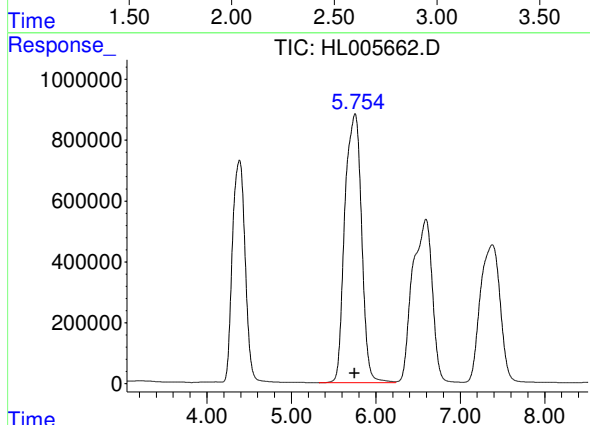


#5 1,3-Dinitrobenzene

R.T.: 5.753 min
Delta R.T.: 0.005 min
Response: 121497366
Conc: 5014.46 ng/ml

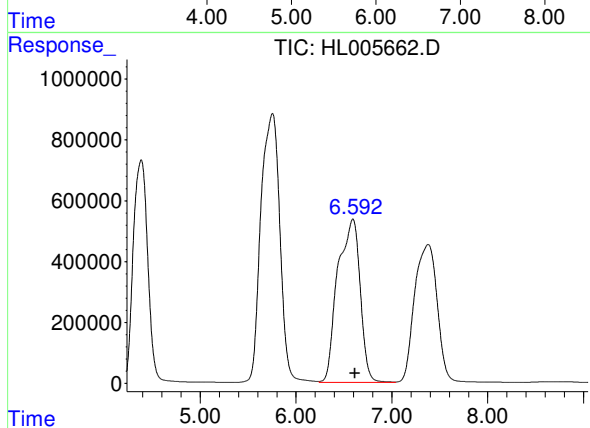

#6 3,5-Dinitroaniline


R.T.: 6.592 min
Delta R.T.: -0.020 min
Response: 87144253
Conc: 5008.37 ug/L

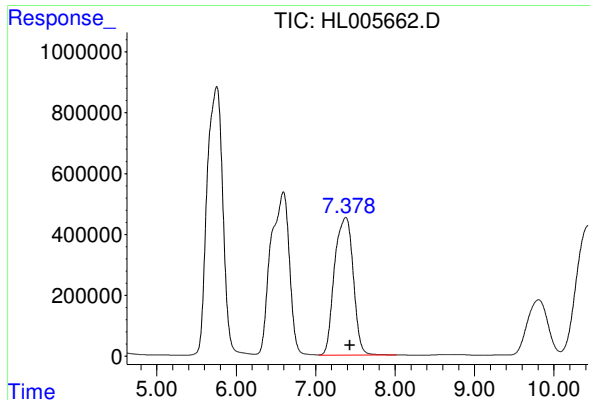

#7 Nitrobenzene

R.T.: 7.377 min
Delta R.T.: -0.056 min
Response: 74040865
Conc: 4996.70 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC5000

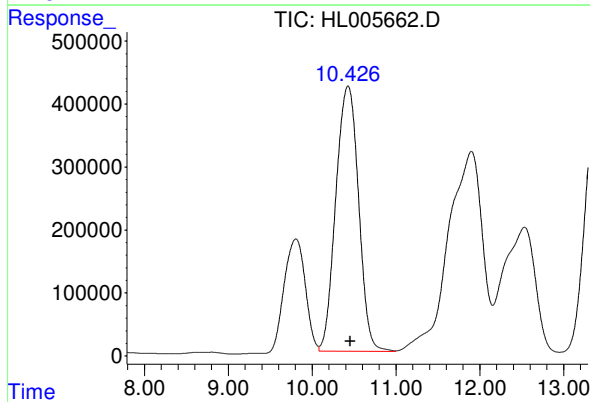

#9 2,4,6-Trinitrotoluene

R.T.: 10.427 min
Delta R.T.: -0.029 min
Response: 79362831
Conc: 5434.99 ug/L