

Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL102214\  
Data File : HL005670.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 22-Oct-2014, 23:03  
Operator : TP  
Sample : HSTDICV0500  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
YS19-SS45-1014

Integration File signal 1: AUTOINT1.E  
Integration File signal 2: autoint2.e  
Quant Time: Mar 11 14:12:04 2015  
Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL102214.M  
Quant Title :  
QLast Update : Mon Mar 09 16:43:57 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T.  | Response | Conc Units    |
|-----------------------------|-------|----------|---------------|
| -----                       |       |          |               |
| System Monitoring Compounds |       |          |               |
| Target Compounds            |       |          |               |
| 5) T 1,3-Dinitrobenzene     | 5.769 | 11483275 | 473.939 ng/ml |
| 6) T 3,5-Dinitroaniline     | 6.597 | 8289903  | 476.439 ug/L  |
| 7) T Nitrobenzene           | 7.386 | 7042934  | 475.297 ug/L  |
| -----                       |       |          |               |

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL102214\  
Data File : HL005670.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 22-Oct-2014, 23:03  
Operator : TP  
Sample : HSTDICV0500  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
YS19-SS45-1014

Integration File signal 1: AUTOINT1.E  
Integration File signal 2: autoint2.e  
Quant Time: Mar 11 14:12:04 2015  
Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL102214.M  
Quant Title :  
QLast Update : Mon Mar 09 16:43:57 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

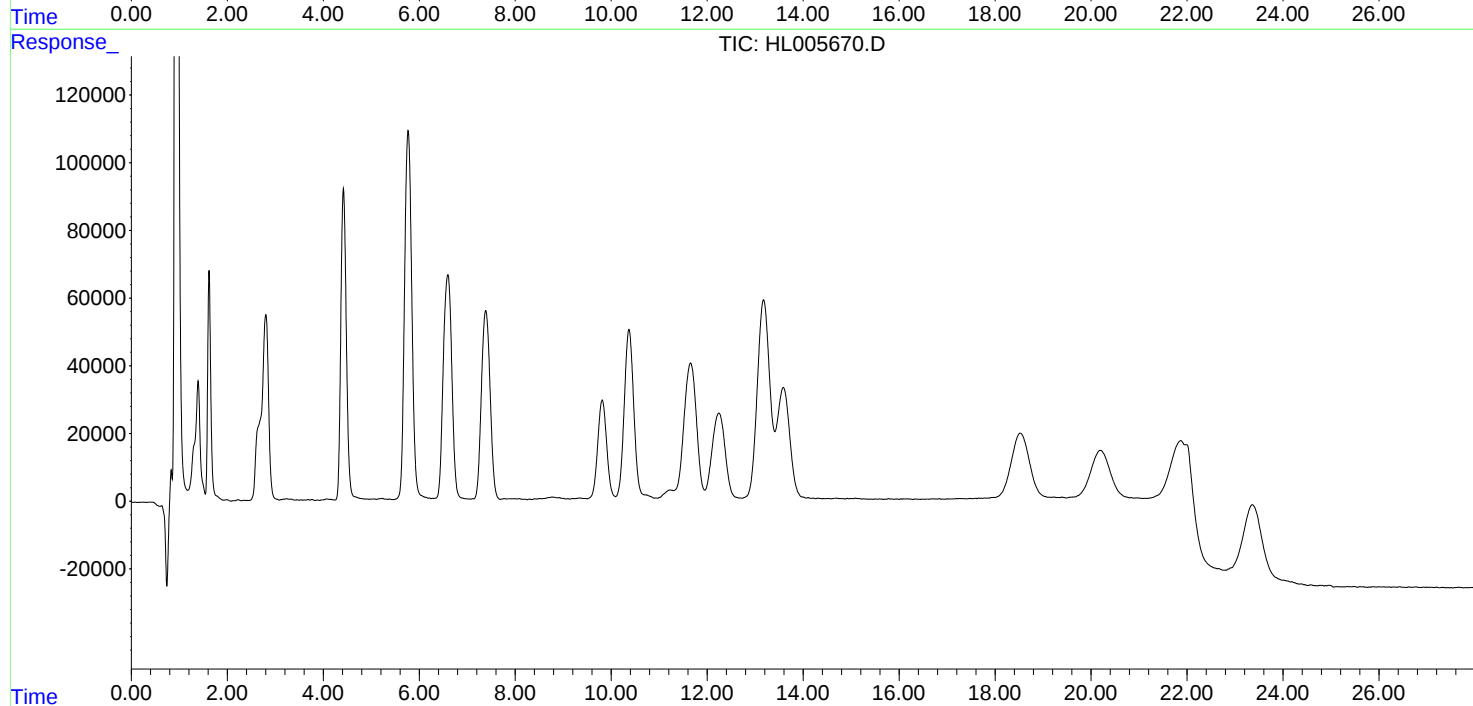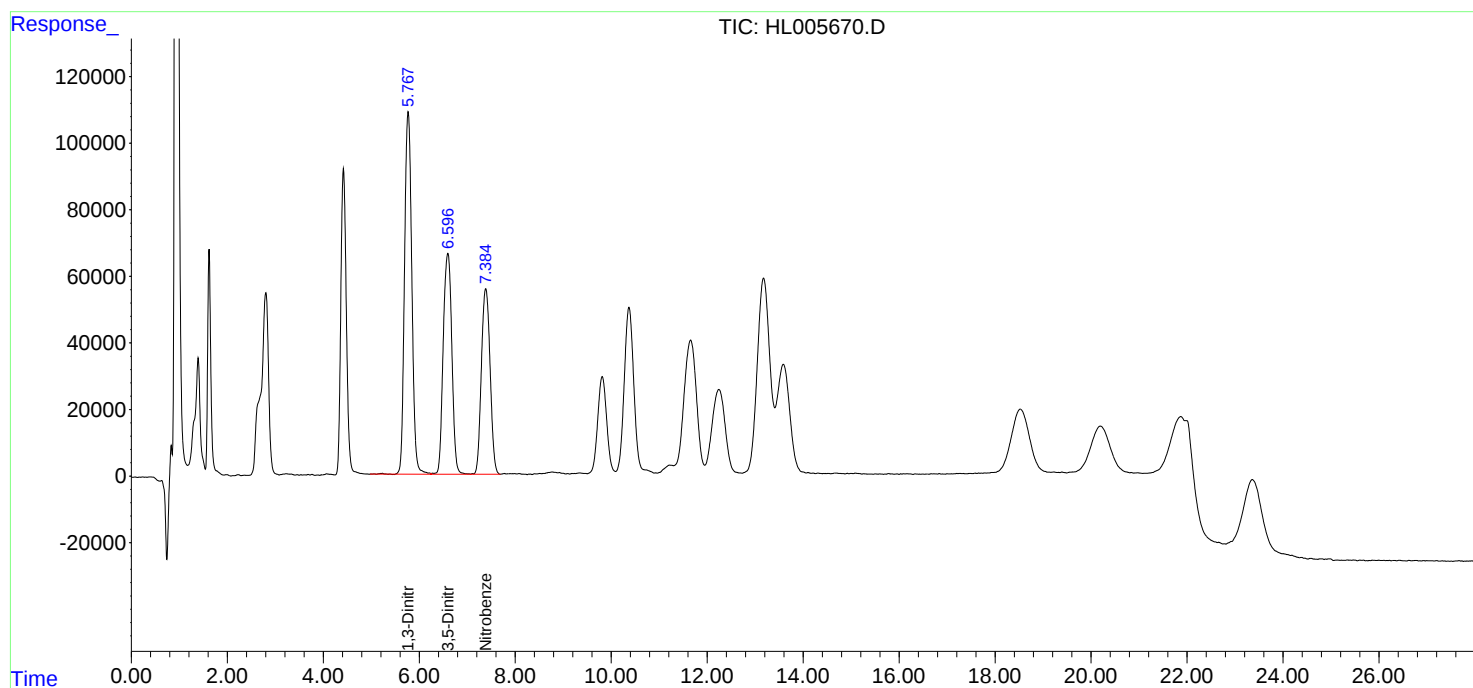


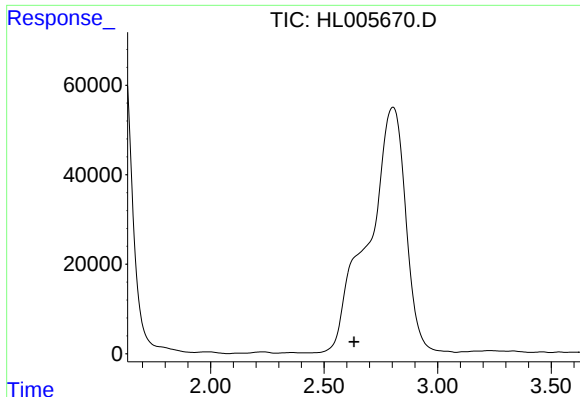

#1 4-Nitroaniline


R.T.: 0.000 min  
Exp R.T.: 2.632 min  
Response: 0  
Conc: N.D.

Instrument :  
HPLC\_L  
ClientSampleId :  
YS19-SS45-1014

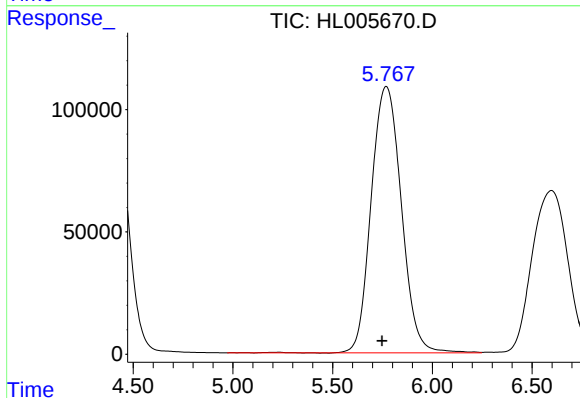


#5 1,3-Dinitrobenzene

R.T.: 5.769 min  
Delta R.T.: 0.021 min  
Response: 11483275  
Conc: 473.94 ng/ml

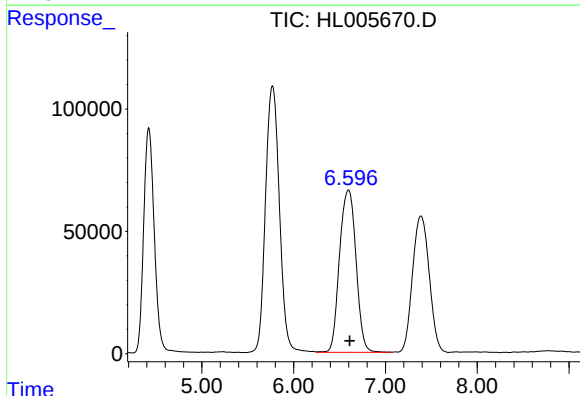

#6 3,5-Dinitroaniline

R.T.: 6.597 min  
Delta R.T.: -0.015 min  
Response: 8289903  
Conc: 476.44 ug/L

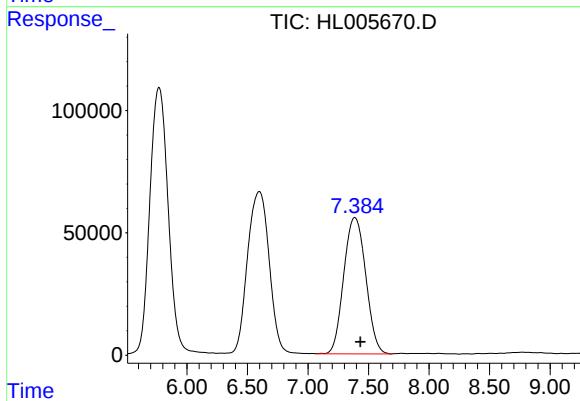

#7 Nitrobenzene

R.T.: 7.386 min  
Delta R.T.: -0.046 min  
Response: 7042934  
Conc: 475.30 ug/L