

Data Path : Z:\HPCHEM1\HPLC_L\HL102214\
Data File : HL005711.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 23-Oct-2014, 19:14
Operator : TP
Sample : HSTDICC001
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0.5

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:54:10 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Quant Title :
QLast Update : Mon Mar 09 16:43:57 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 uL
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\HL102214\
Data File : HL005711.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 23-Oct-2014, 19:14
Operator : TP
Sample : HSTDICC001
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0.5

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:54:10 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Quant Title :
QLast Update : Mon Mar 09 16:43:57 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

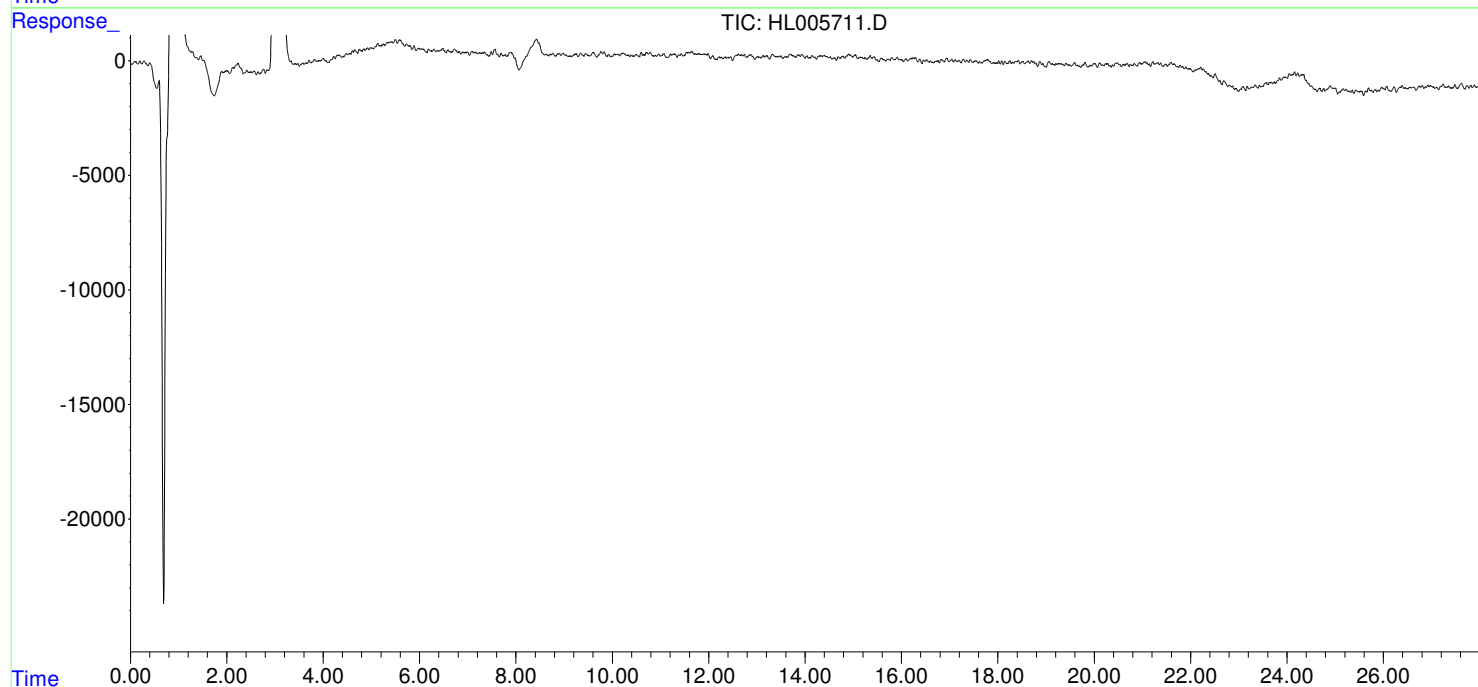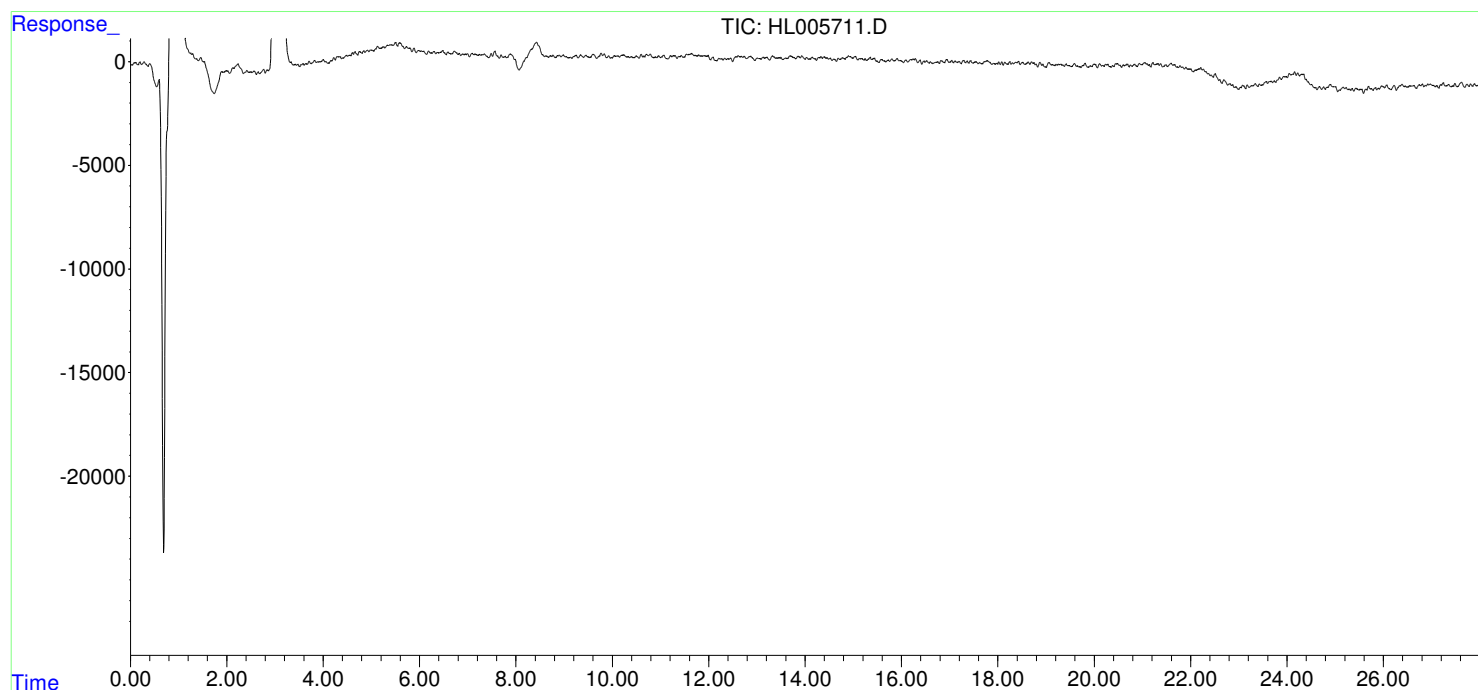

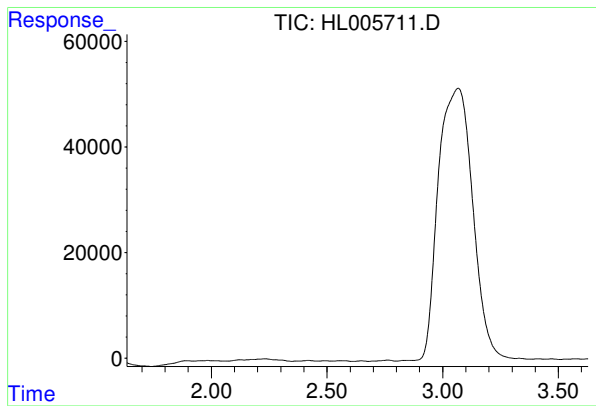

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 2.632 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0.5