

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL102214\
 Data File : HL005668.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 22-Oct-2014, 22:04
 Operator : TP
 Sample : HSTDICCC0500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDICCC0500

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 04:31:22 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
 Quant Title :
 QLast Update : Sun Mar 08 04:30:45 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.641	5941239	500.000 ug/L
Target Compounds			
2) T HMX	1.515	2767749	500.000 ug/L
3) T RDX	2.641	5941239	500.000 ug/L
4) T 1,3,5-Trinitrobenzene	4.251	7371338	500.000 ug/L
5) T 1,3-Dinitrobenzene	5.593	11163534	500.000 ng/ml
6) T 3,5-Dinitroaniline	6.422	8079258	500.000 ug/L
7) T Nitrobenzene	7.206	6828794	500.000 ug/L
8) T Tetryl	9.605	4777368	500.000 ug/L
9) T 2,4,6-Trinitrotoluene	10.165	7131528	500.000 ug/L
10) T 2-Amino-4,6-dinitroto...	11.463	7576412	500.000 ug/L
11) T 4-Amino-2,6-dinitroto...	12.049	4811217	500.000 ug/L
12) T 2,4-Dinitrotoluene	12.986	10598669	500.000 ug/L
13) T 2,6-Dinitrotoluene	13.394	5710725	500.000 ug/L
14) T 2-Nitrotoluene	18.304	4913046	500.000 ug/L
15) T 4-Nitrotoluene	19.964	3873930	500.000 ug/L
16) T 3-Nitrotoluene	21.629	5569371	500.000 ug/L
17) T PETN	23.133	5453059	500.000 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL102214\
Data File : HL005668.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 22-Oct-2014, 22:04
Operator : TP
Sample : HSTDICCC0500
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDICCC0500

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 08 04:31:22 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Quant Title :
QLast Update : Sun Mar 08 04:30:45 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

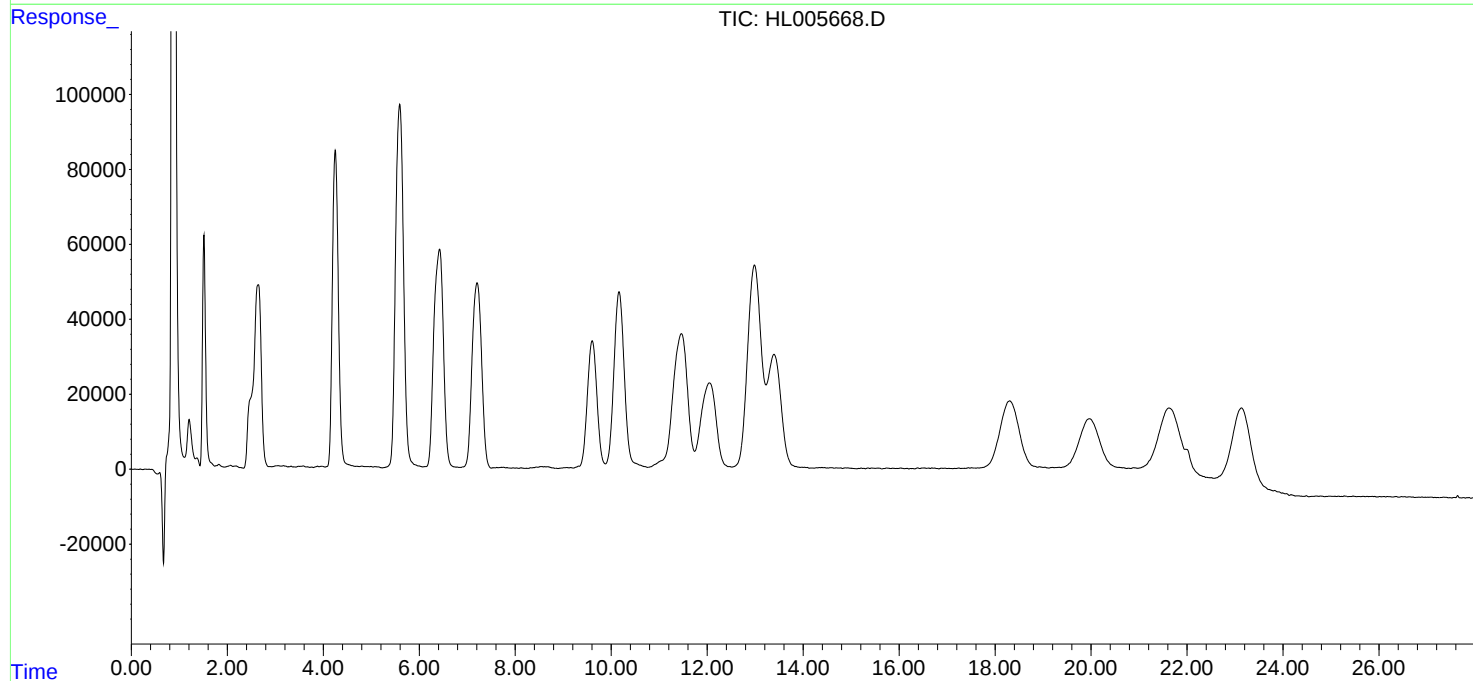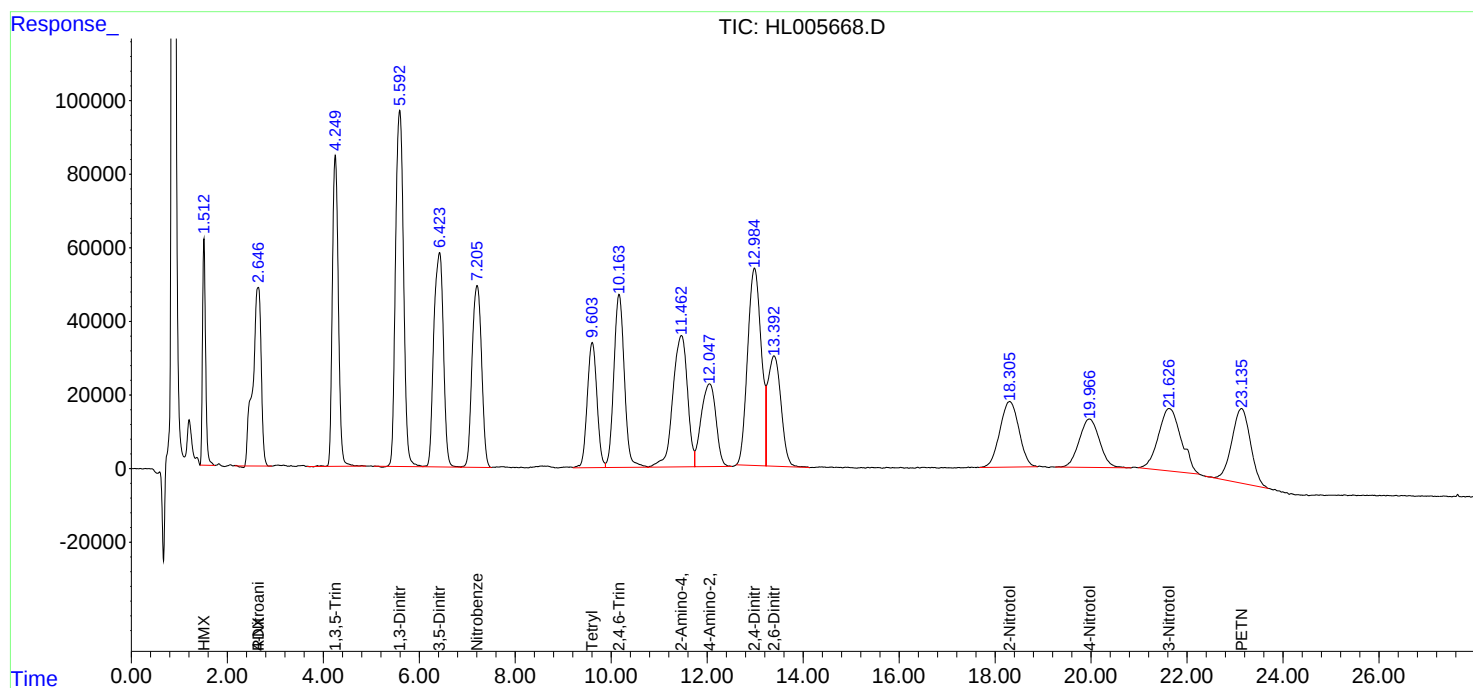


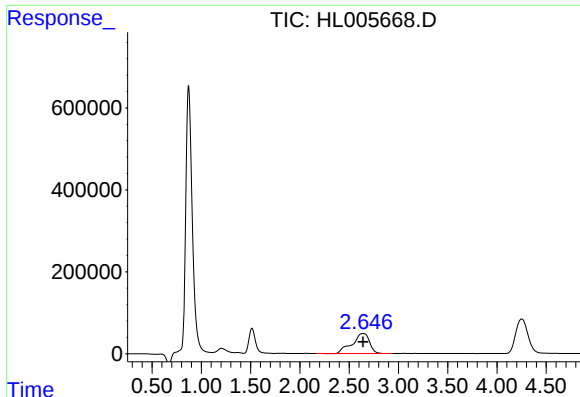

#1 4-Nitroaniline


R.T.: 2.641 min
Delta R.T.: 0.000 min
Response: 5941239
Conc: 500.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0500

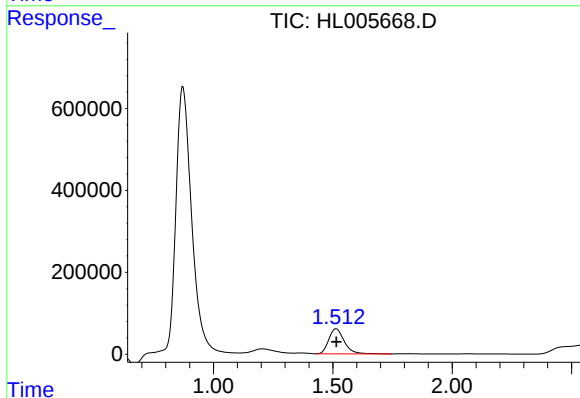


#2 HMX

R.T.: 1.515 min
Delta R.T.: 0.000 min
Response: 2767749
Conc: 500.00 ug/L

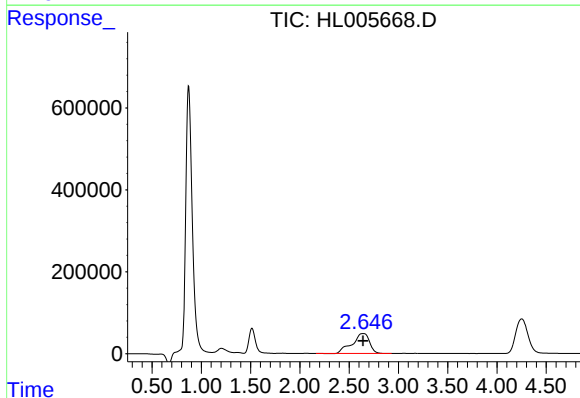


#3 RDX

R.T.: 2.641 min
Delta R.T.: 0.000 min
Response: 5941239
Conc: 500.00 ug/L

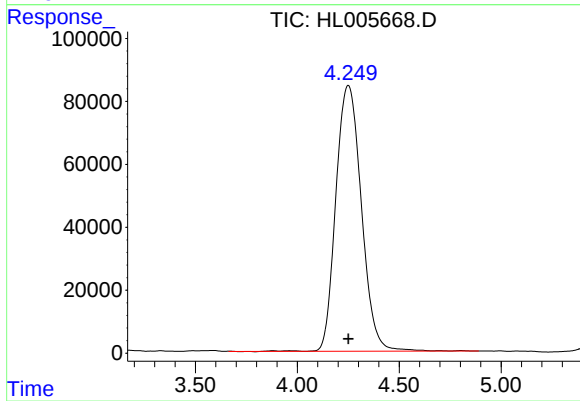

#4 1,3,5-Trinitrobenzene


R.T.: 4.251 min
Delta R.T.: 0.000 min
Response: 7371338
Conc: 500.00 ug/L

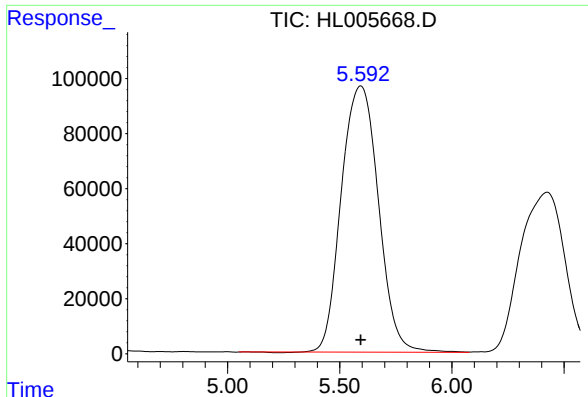

#5 1,3-Dinitrobenzene


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 11163534
Conc: 500.00 ng/ml

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0500

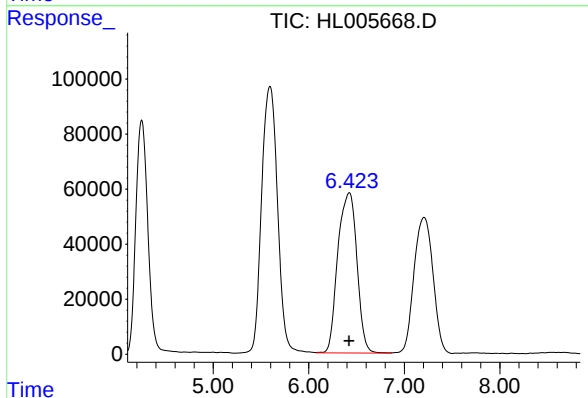


#6 3,5-Dinitroaniline

R.T.: 6.422 min
Delta R.T.: 0.000 min
Response: 8079258
Conc: 500.00 ug/L

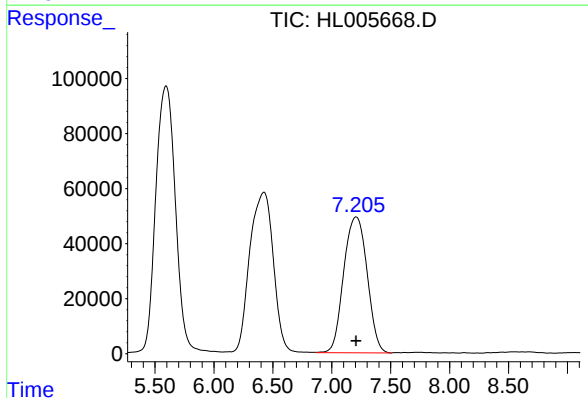


#7 Nitrobenzene

R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 6828794
Conc: 500.00 ug/L

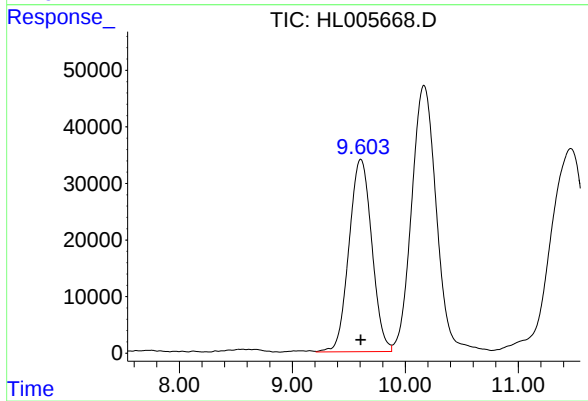

#8 Tetryl


R.T.: 9.605 min
Delta R.T.: 0.000 min
Response: 4777368
Conc: 500.00 ug/L

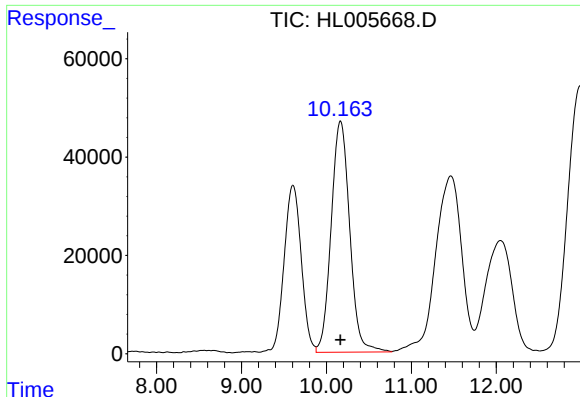

#9 2,4,6-Trinitrotoluene


R.T.: 10.165 min
Delta R.T.: 0.000 min
Response: 7131528
Conc: 500.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0500

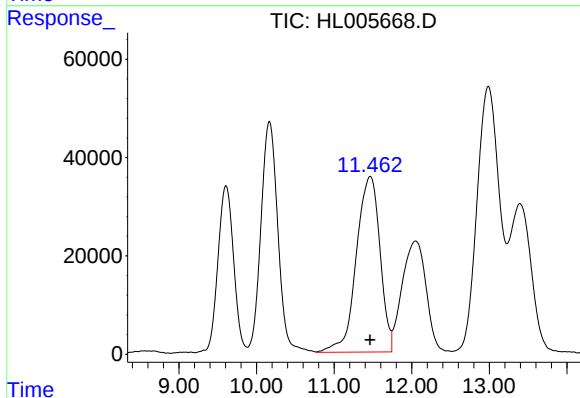


#10 2-Amino-4,6-dinitrotoluene

R.T.: 11.463 min
Delta R.T.: 0.000 min
Response: 7576412
Conc: 500.00 ug/L

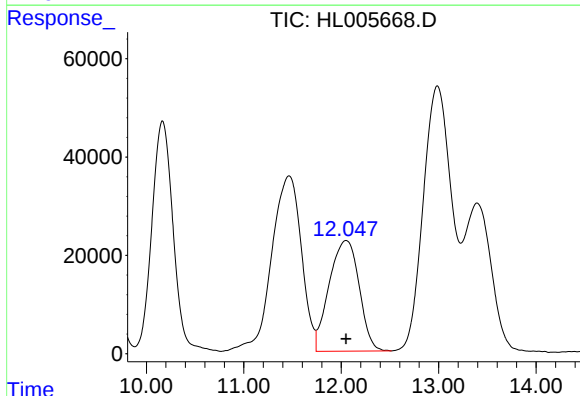


#11 4-Amino-2,6-dinitrotoluene

R.T.: 12.049 min
Delta R.T.: 0.000 min
Response: 4811217
Conc: 500.00 ug/L

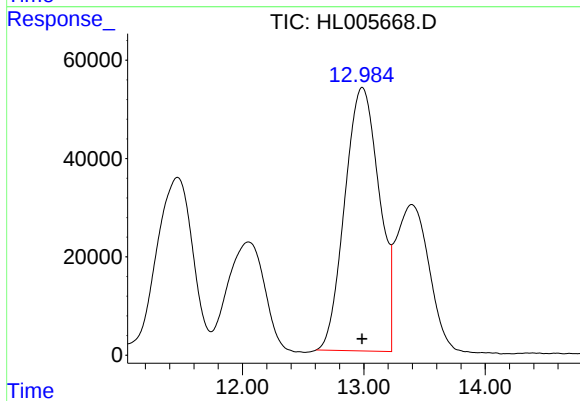

#12 2,4-Dinitrotoluene


R.T.: 12.986 min
Delta R.T.: 0.000 min
Response: 10598669
Conc: 500.00 ug/L

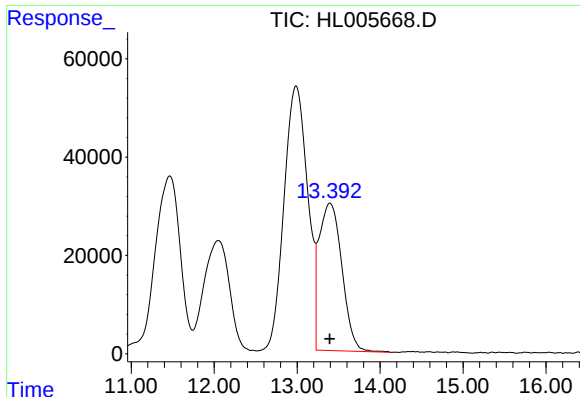

#13 2,6-Dinitrotoluene


R.T.: 13.394 min
Delta R.T.: 0.000 min
Response: 5710725
Conc: 500.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0500

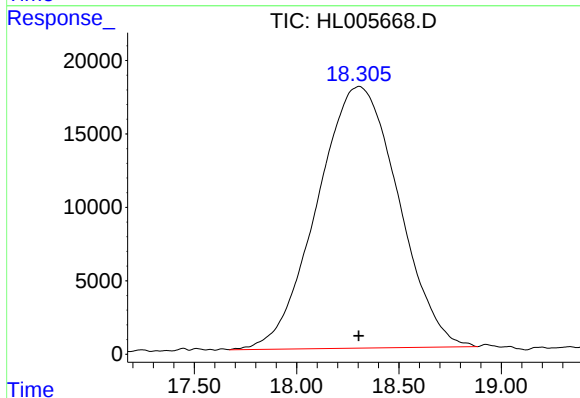


#14 2-Nitrotoluene

R.T.: 18.304 min
Delta R.T.: 0.000 min
Response: 4913046
Conc: 500.00 ug/L

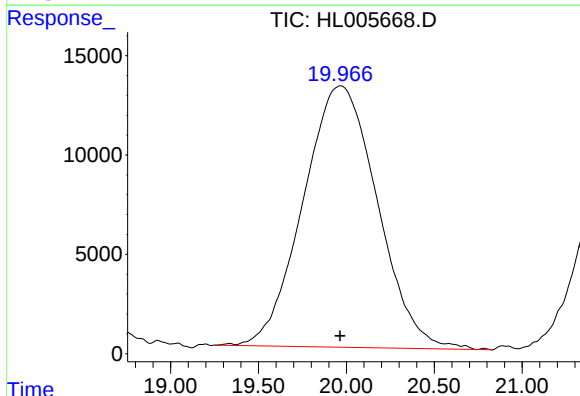


#15 4-Nitrotoluene

R.T.: 19.964 min
Delta R.T.: 0.000 min
Response: 3873930
Conc: 500.00 ug/L

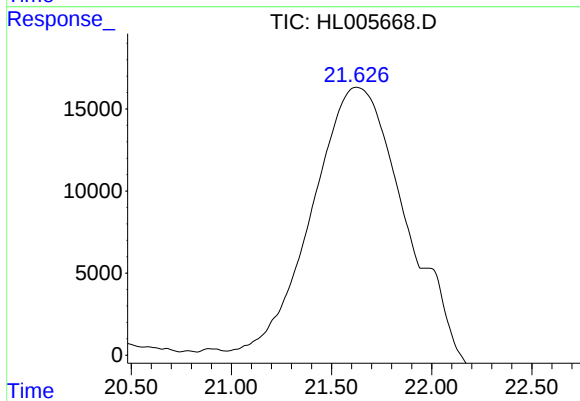

#16 3-Nitrotoluene

R.T.: 21.629 min
Delta R.T.: 0.000 min
Response: 5569371
Conc: 500.00 ug/L

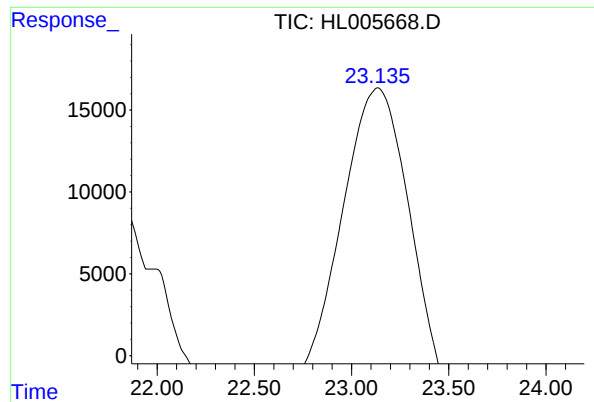

#17 PETN

R.T.: 23.133 min
Delta R.T.: 0.000 min
Response: 5453059
Conc: 500.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDICC0500