

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL102214\
 Data File : HL005676.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 23-Oct-2014, 01:59
 Operator : TP
 Sample : F4222-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 YS19-GW03-1014

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 14:26:17 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
 Quant Title :
 QLast Update : Sun Mar 08 14:26:07 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.513	1968890	151.844 ug/L
Target Compounds			
6) T 3,5-Dinitroaniline	6.684	1824445	104.855 ug/L
9) T 2,4,6-Trinitrotoluene	10.545	15469667	1059.407 ug/L
10) T 2-Amino-4,6-dinitroto...	11.841	6905006	424.151 ug/L
11) T 4-Amino-2,6-dinitroto...	12.431	15156554	1480.330 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL102214\
Data File : HL005676.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 23-Oct-2014, 01:59
Operator : TP
Sample : F4222-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
YS19-GW03-1014

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 08 14:26:17 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Quant Title :
QLast Update : Sun Mar 08 14:26:07 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

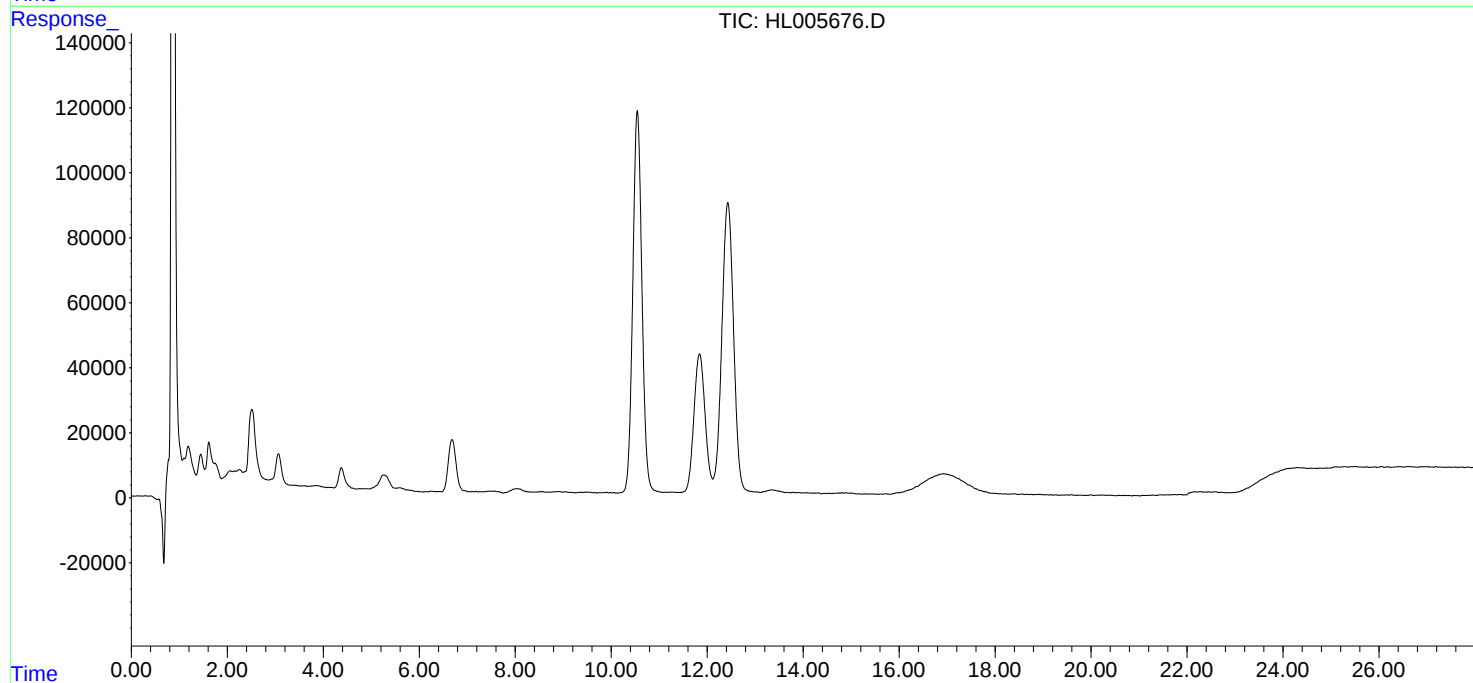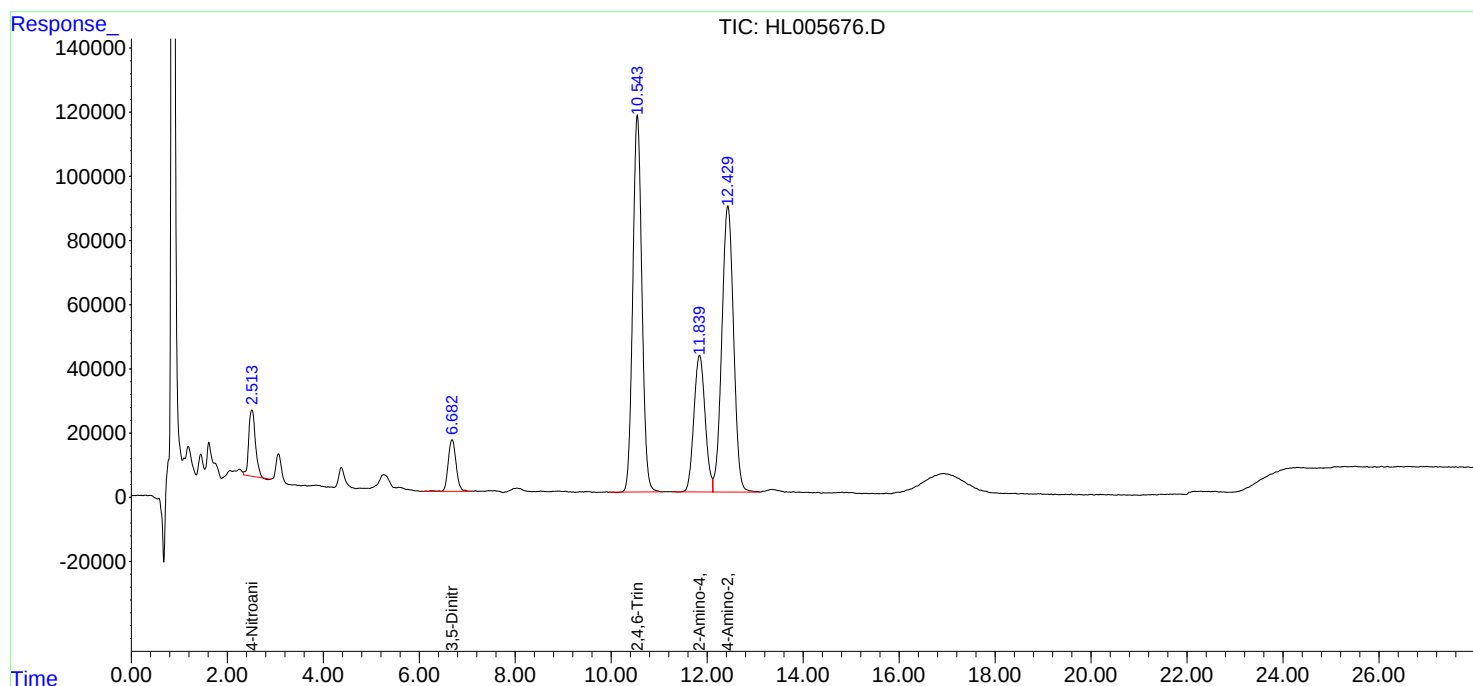


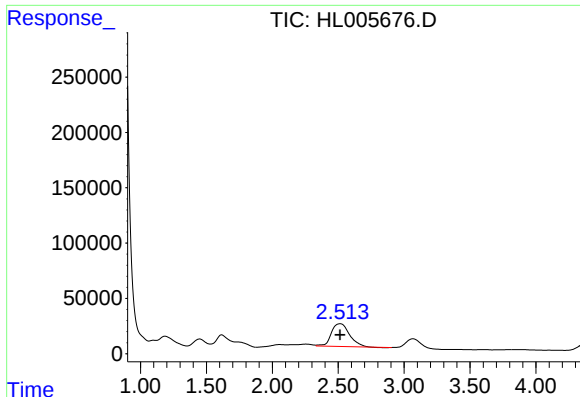

#1 4-Nitroaniline


R.T.: 2.513 min
Delta R.T.: 0.000 min
Response: 1968890
Conc: 151.84 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-GW03-1014

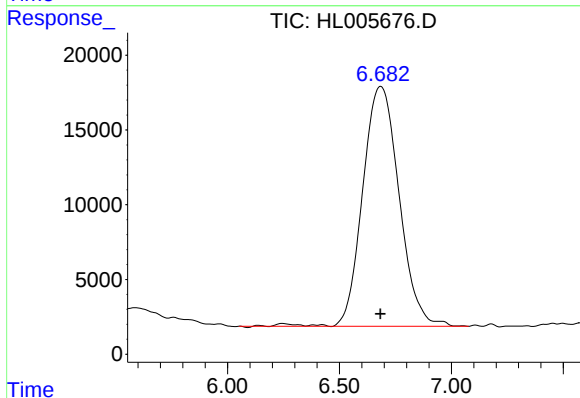


#6 3,5-Dinitroaniline

R.T.: 6.684 min
Delta R.T.: 0.002 min
Response: 1824445
Conc: 104.85 ug/L

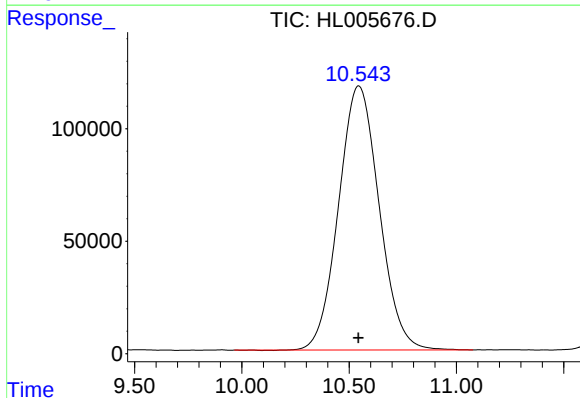


#9 2,4,6-Trinitrotoluene

R.T.: 10.545 min
Delta R.T.: 0.002 min
Response: 15469667
Conc: 1059.41 ug/L

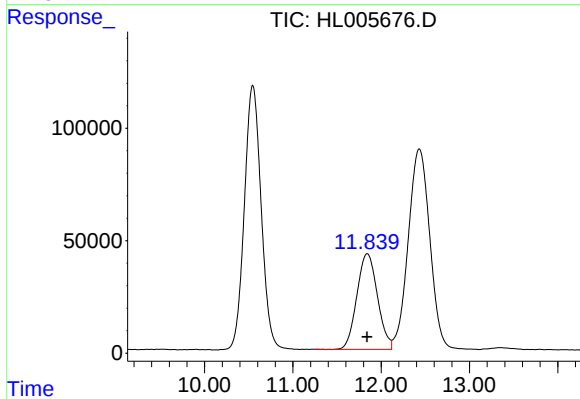

#10 2-Amino-4,6-dinitrotoluene

R.T.: 11.841 min
Delta R.T.: 0.002 min
Response: 6905006
Conc: 424.15 ug/L

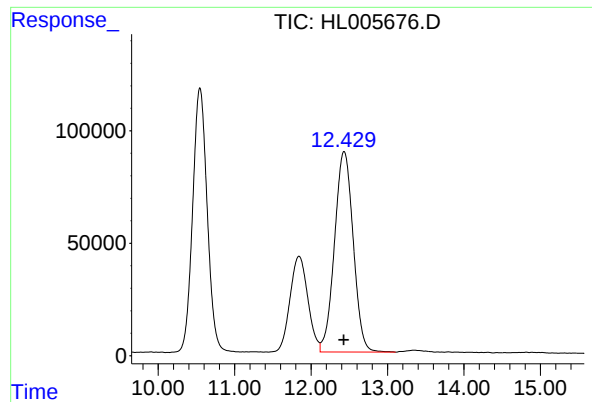

#11 4-Amino-2,6-dinitrotoluene

R.T.: 12.431 min
Delta R.T.: 0.002 min
Response: 15156554
Conc: 1480.33 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-GW03-1014