

Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL102214\  
Data File : HL005686.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 23-Oct-2014, 06:53  
Operator : TP  
Sample : F4303-12  
Misc :  
ALS Vial : 28 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
YS19-SB03-1014

Integration File signal 1: AUTOINT1.E  
Integration File signal 2: autoint2.e  
Quant Time: Mar 08 07:13:48 2015  
Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL102214.M  
Quant Title :  
QLast Update : Sun Mar 08 07:02:15 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T.  | Response | Conc Units  |
|-----------------------------|-------|----------|-------------|
| -----                       |       |          |             |
| System Monitoring Compounds |       |          |             |
| 1) S 4-Nitroaniline         | 2.504 | 993912   | 76.652 ug/L |
| Target Compounds            |       |          |             |
| -----                       |       |          |             |

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_L\Data\HL102214\  
Data File : HL005686.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 23-Oct-2014, 06:53  
Operator : TP  
Sample : F4303-12  
Misc :  
ALS Vial : 28 Sample Multiplier: 1

Instrument :  
HPLC\_L  
ClientSampleId :  
YS19-SB03-1014

Integration File signal 1: AUTOINT1.E  
Integration File signal 2: autoint2.e  
Quant Time: Mar 08 07:13:48 2015  
Quant Method : Z:\HPCHEM1\HPLC\_L\METHODS\HL102214.M  
Quant Title :  
QLast Update : Sun Mar 08 07:02:15 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

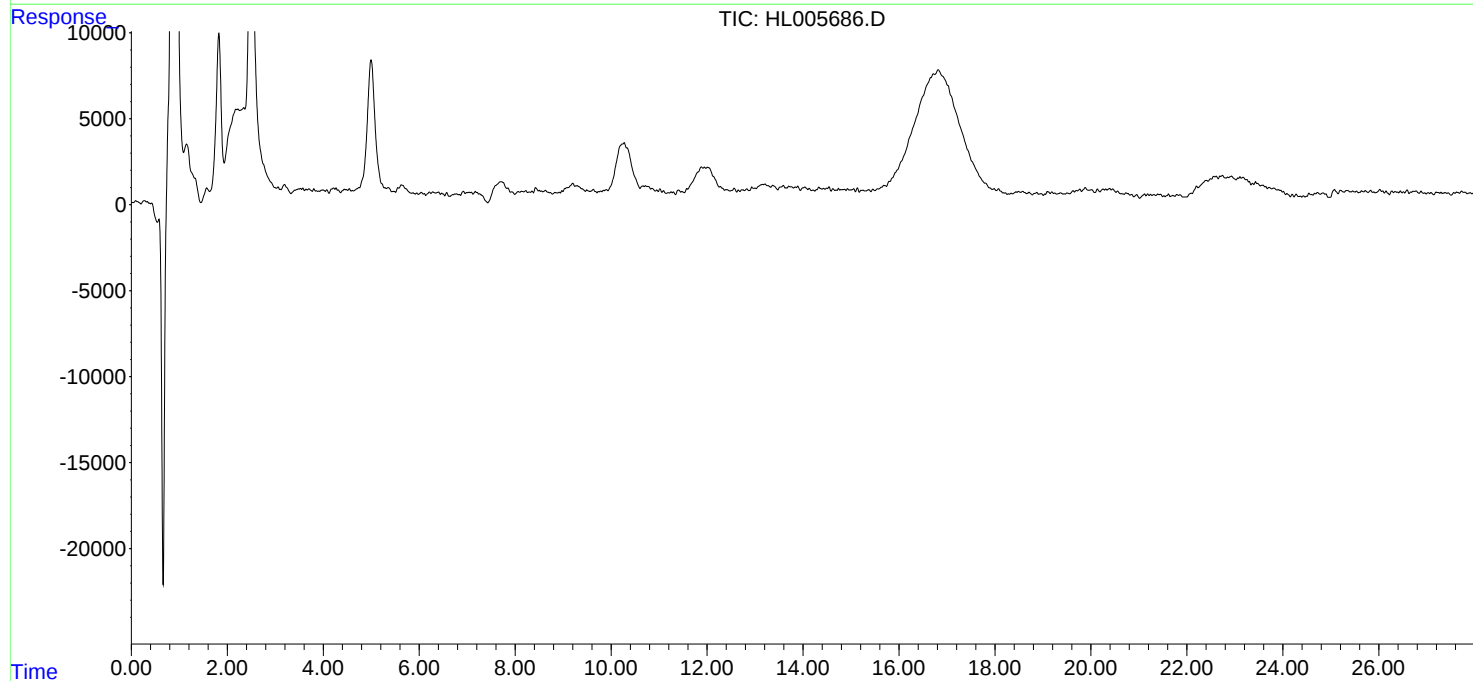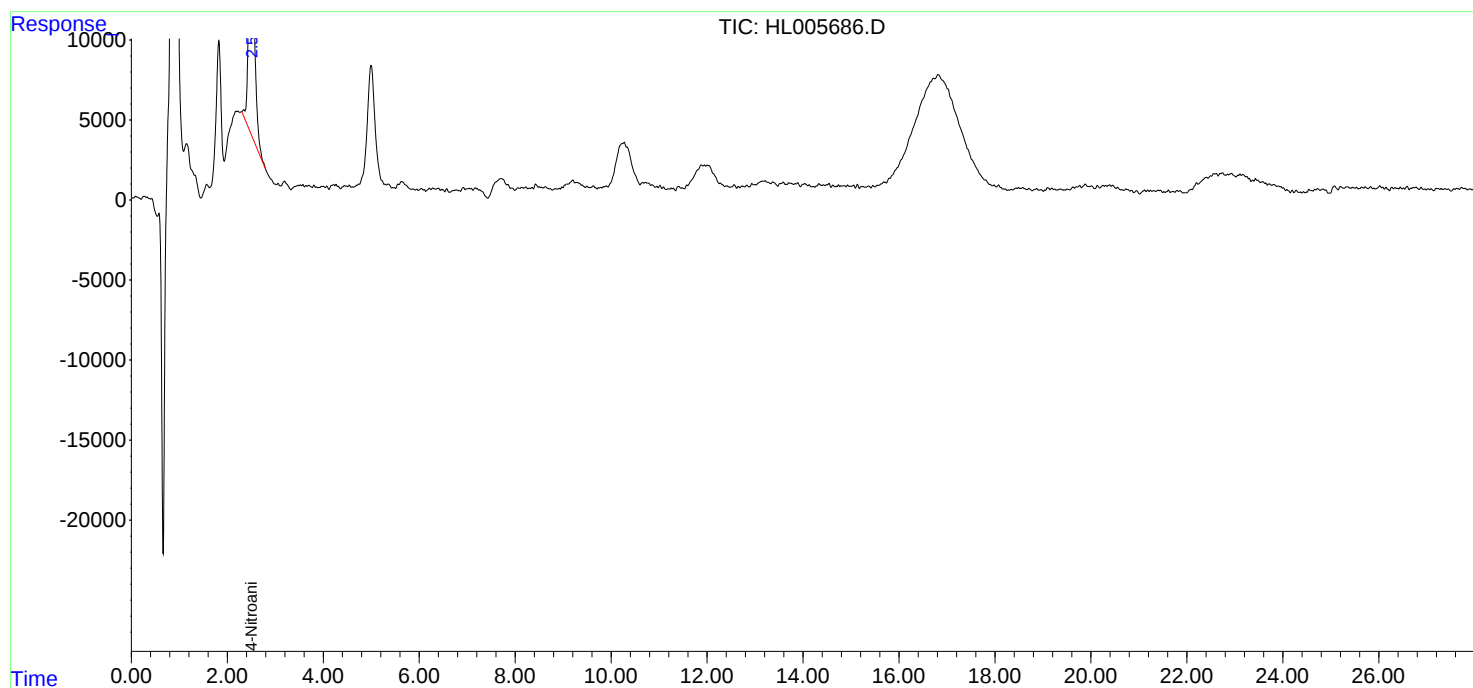

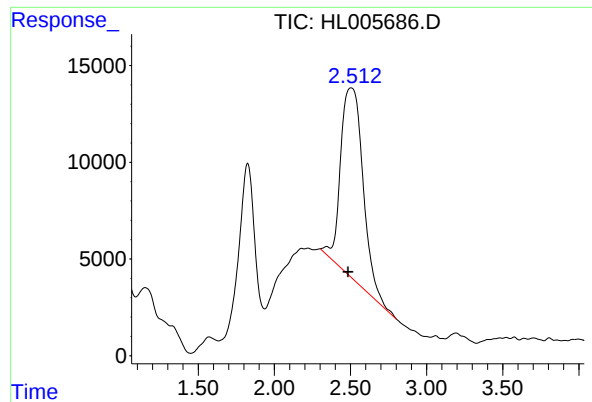

#1 4-Nitroaniline

R.T.: 2.504 min  
Delta R.T.: 0.021 min  
Response: 993912  
Conc: 76.65 ug/L

Instrument :  
HPLC\_L  
ClientSampleId :  
YS19-SB03-1014