

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005827.D Vial: 5
Acq On : 04-Nov-2014, 17:07 Operator: TP
Sample : F4368-07 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 5 4:00 2014 Quant Results File: HL102214.RES

Instrument :
HPLC_L
ClientSampleId :
YS19-SS40-1014

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Title :
Last Update : Fri Oct 25 15:16:02 2013
Response via : Initial Calibration
DataAcq Meth : TEST.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) T RDX	2.18	415031	41.667 ug/L

Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.


HL005827.D HL102214.M Wed Nov 05 03:57:33 2014


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005827.D Vial: 5
Acq On : 04-Nov-2014, 17:07 Operator: TP
Sample : F4368-07 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 5 4:00 2014 Quant Results File: HL102214.RES

Instrument :
HPLC_L
ClientSampleId :
YS19-SS40-1014

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Title :
Last Update : Fri Oct 25 15:16:02 2013
Response via : Multiple Level Calibration
DataAcq Meth : TEST.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

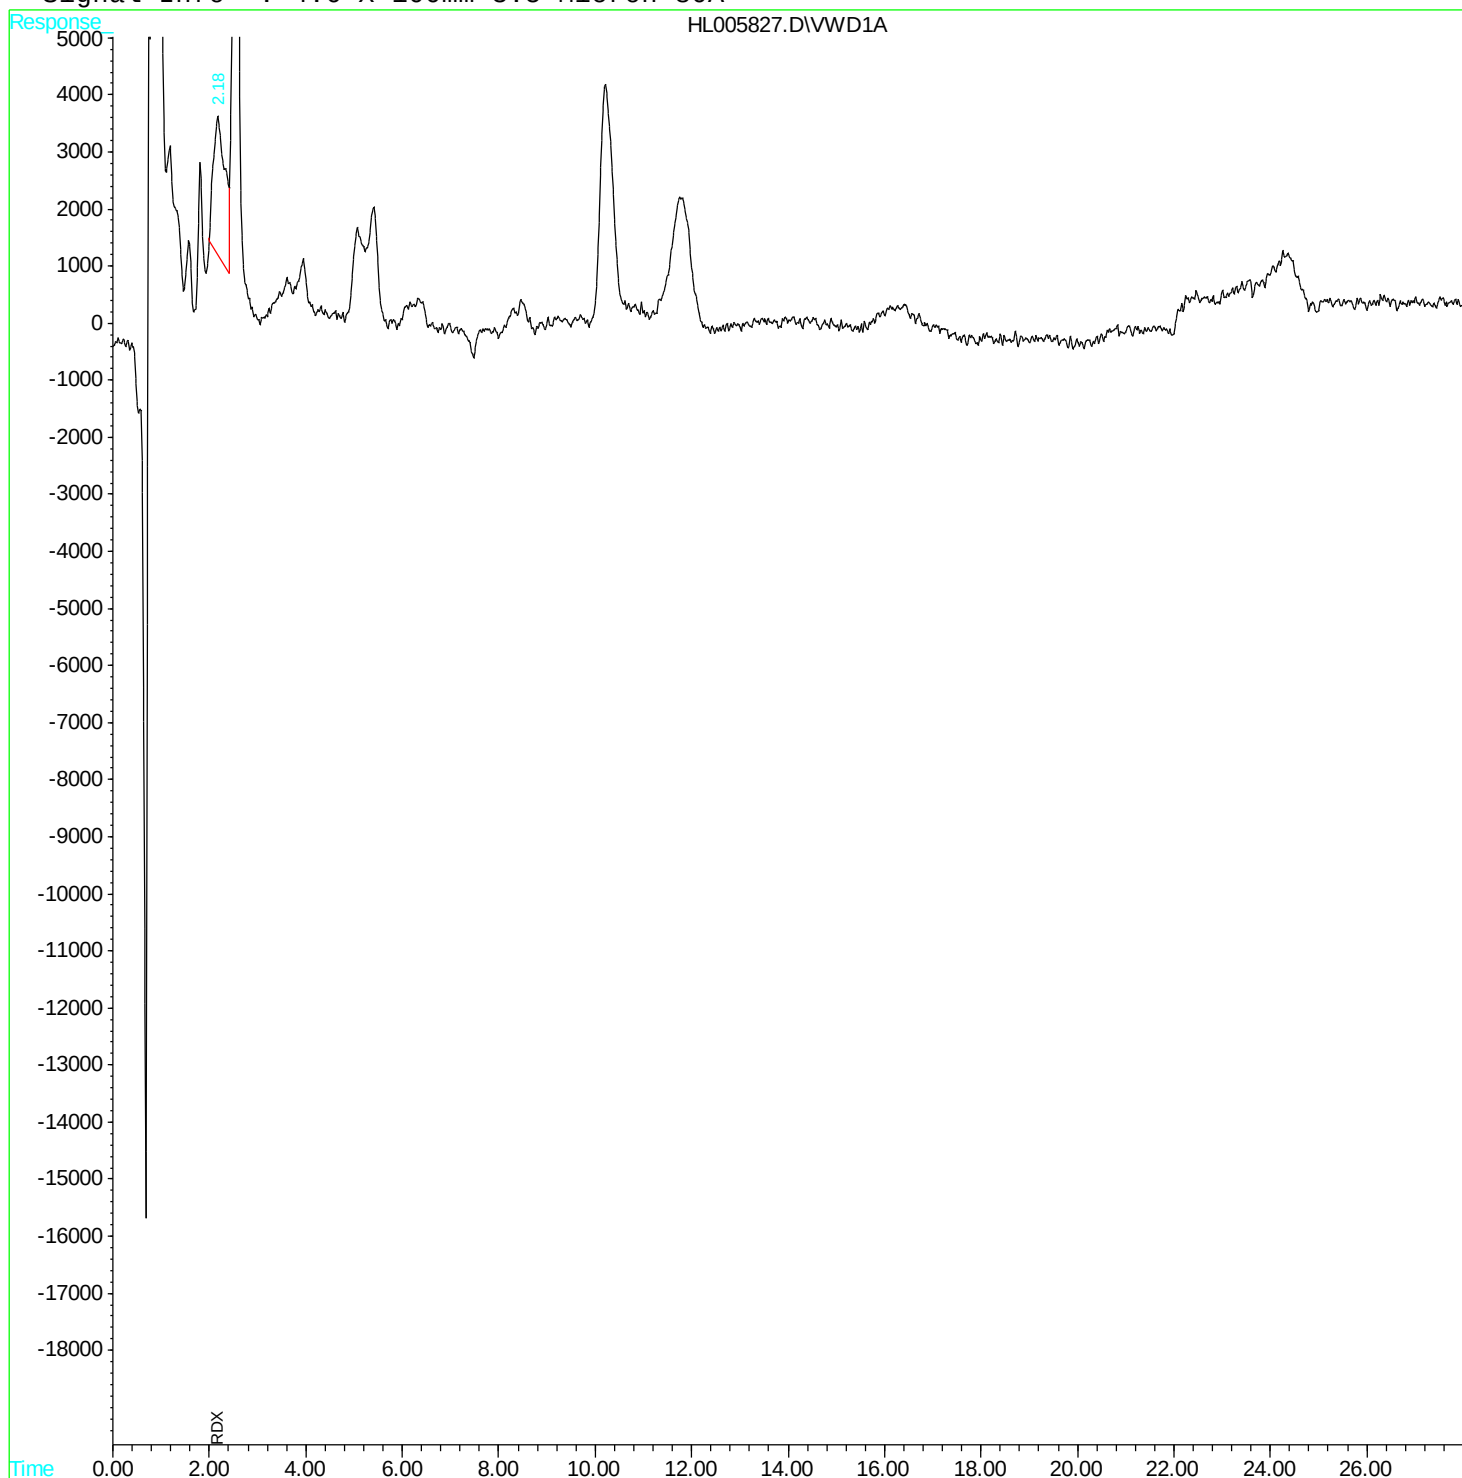


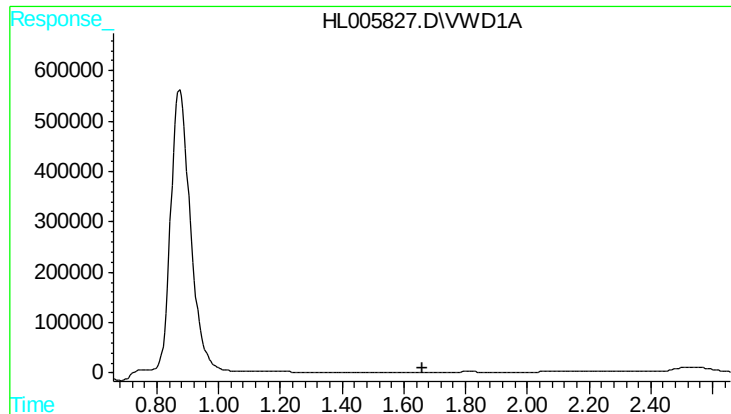

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 1.659 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
YS19-SS40-1014

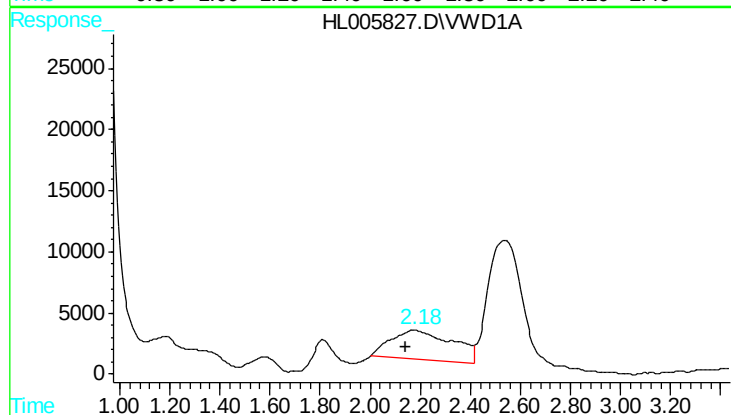

#3 RDX

R.T.: 2.177 min
Delta R.T.: 0.033 min
Response: 415031
Conc: 41.67 ug/L