

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005831.D Vial: 9
Acq On : 04-Nov-2014, 19:04 Operator: TP
Sample : F4368-16 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 5 4:00 2014 Quant Results File: HL102214.RES

Instrument :
HPLC_L
ClientSampleId :
YS19-SS44-1014

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Title :
Last Update : Fri Oct 25 15:16:02 2013
Response via : Initial Calibration
DataAcq Meth : TEST.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13) T	2,6-Dinitrotoluene	11.90	907102	77.898 ug/L
-------	--------------------	-------	--------	-------------

Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.

HL005831.D HL102214.M Wed Nov 05 03:57:51 2014


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005831.D Vial: 9
 Acq On : 04-Nov-2014, 19:04 Operator: TP
 Sample : F4368-16 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : AUTOINT1.E
 Quant Time: Nov 5 4:00 2014 Quant Results File: HL102214.RES

Instrument :
 HPLC_L
 ClientSampleId :
 YS19-SS44-1014

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
 Title :
 Last Update : Fri Oct 25 15:16:02 2013
 Response via : Multiple Level Calibration
 DataAcq Meth : TEST.M

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

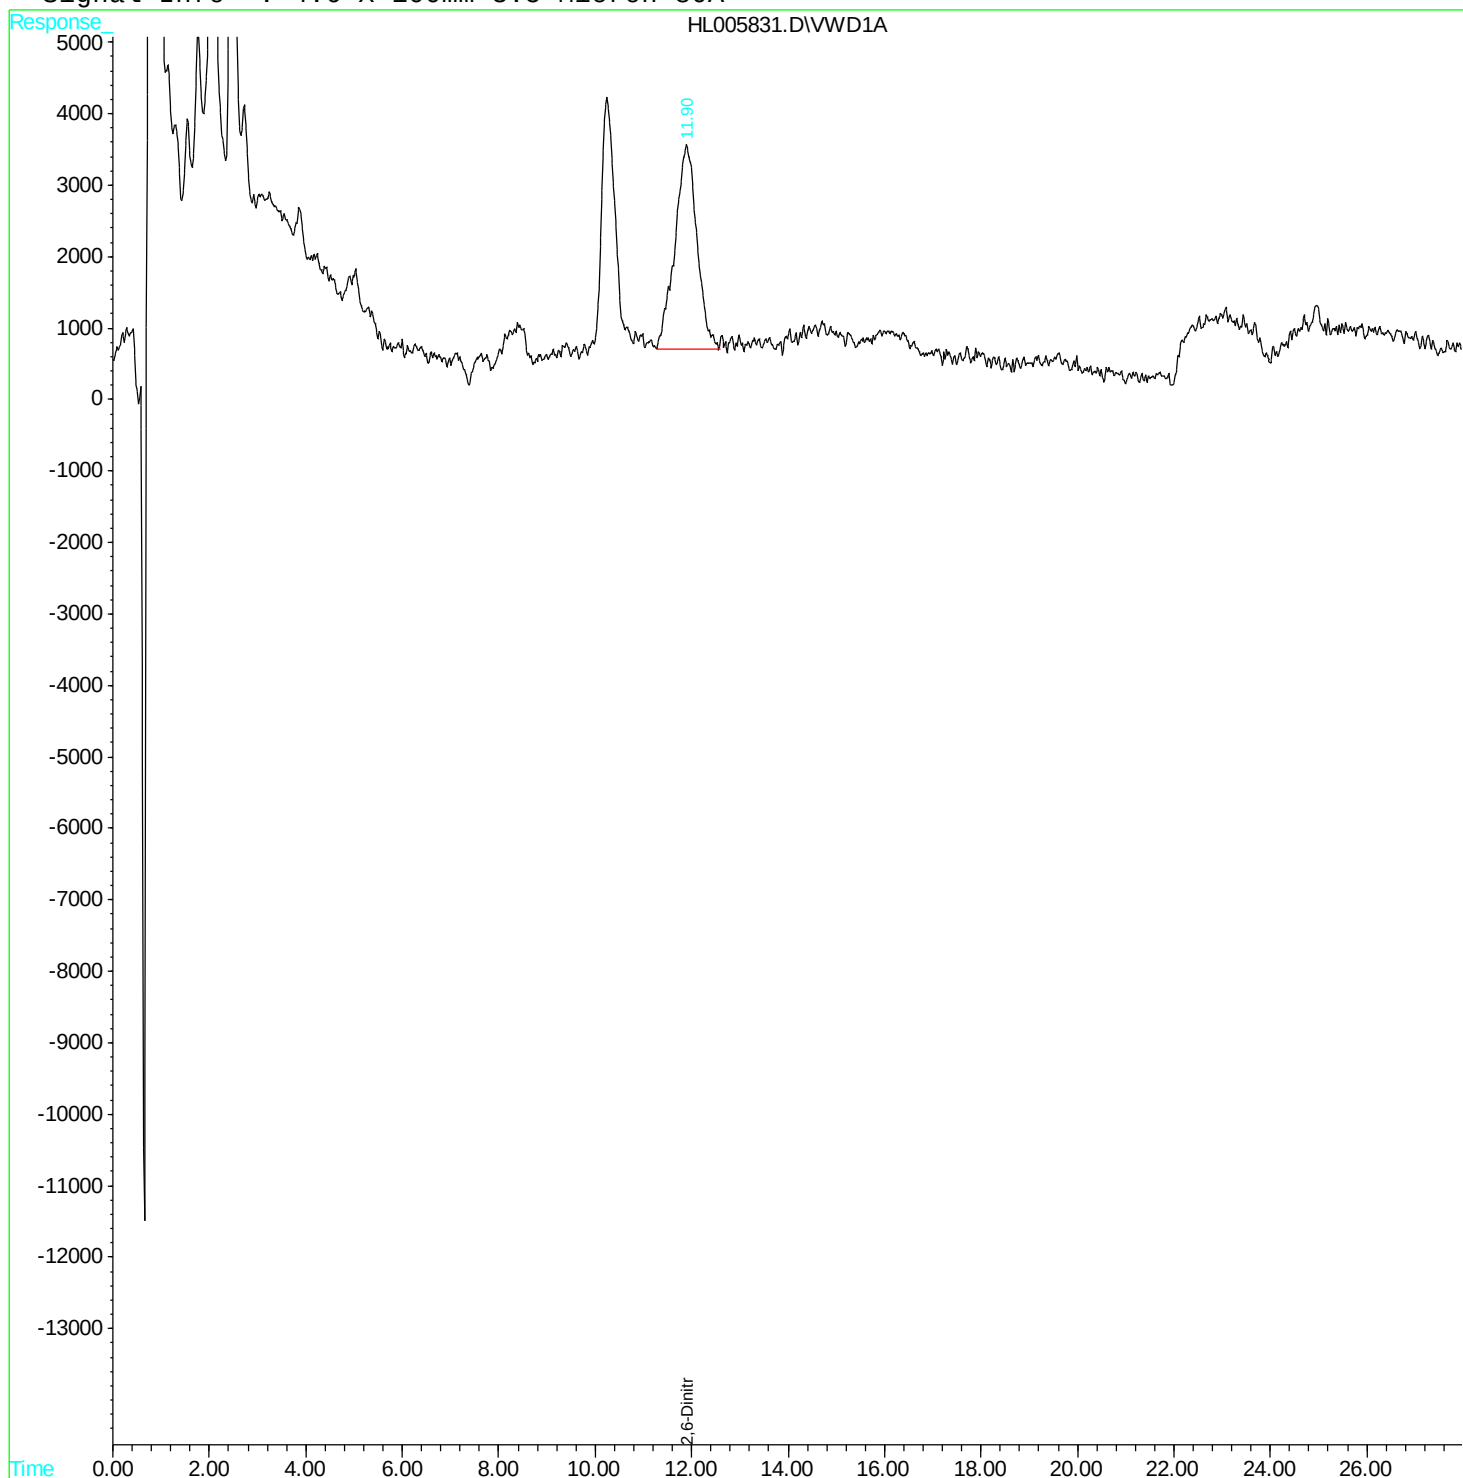


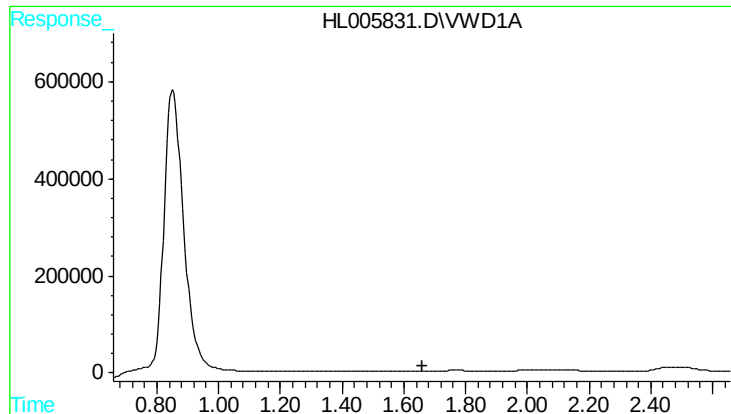

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 1.659 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
YS19-SS44-1014

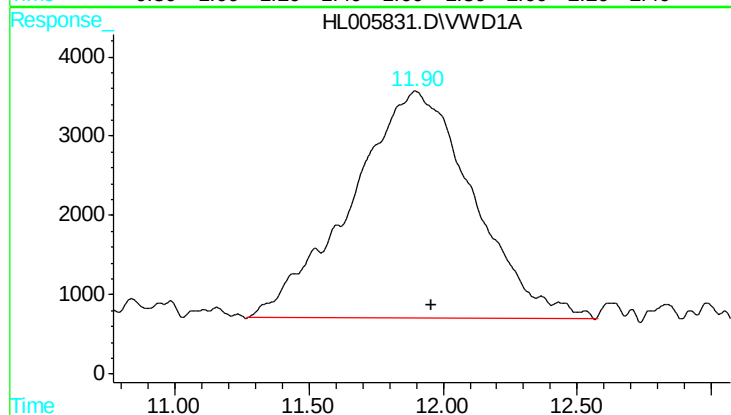

#13 2,6-Dinitrotoluene

R.T.: 11.898 min
Delta R.T.: -0.061 min
Response: 907102
Conc: 77.90 ug/L