

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005834.D Vial: 1
Acq On : 04-Nov-2014, 20:32 Operator: TP
Sample : HSTDCCC0500 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 5 4:00 2014 Quant Results File: HL102214.RES

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Title :
Last Update : Fri Oct 25 15:16:02 2013
Response via : Initial Calibration
DataAcq Meth : TEST.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13) T	2,6-Dinitrotoluene	11.92	4776899	410.218 ug/L
-------	--------------------	-------	---------	--------------

Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.


HL005834.D HL102214.M Wed Nov 05 03:58:05 2014


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005834.D Vial: 1
Acq On : 04-Nov-2014, 20:32 Operator: TP
Sample : HSTDCCC0500 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 5 4:00 2014 Quant Results File: HL102214.RES

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Title :
Last Update : Fri Oct 25 15:16:02 2013
Response via : Multiple Level Calibration
DataAcq Meth : TEST.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

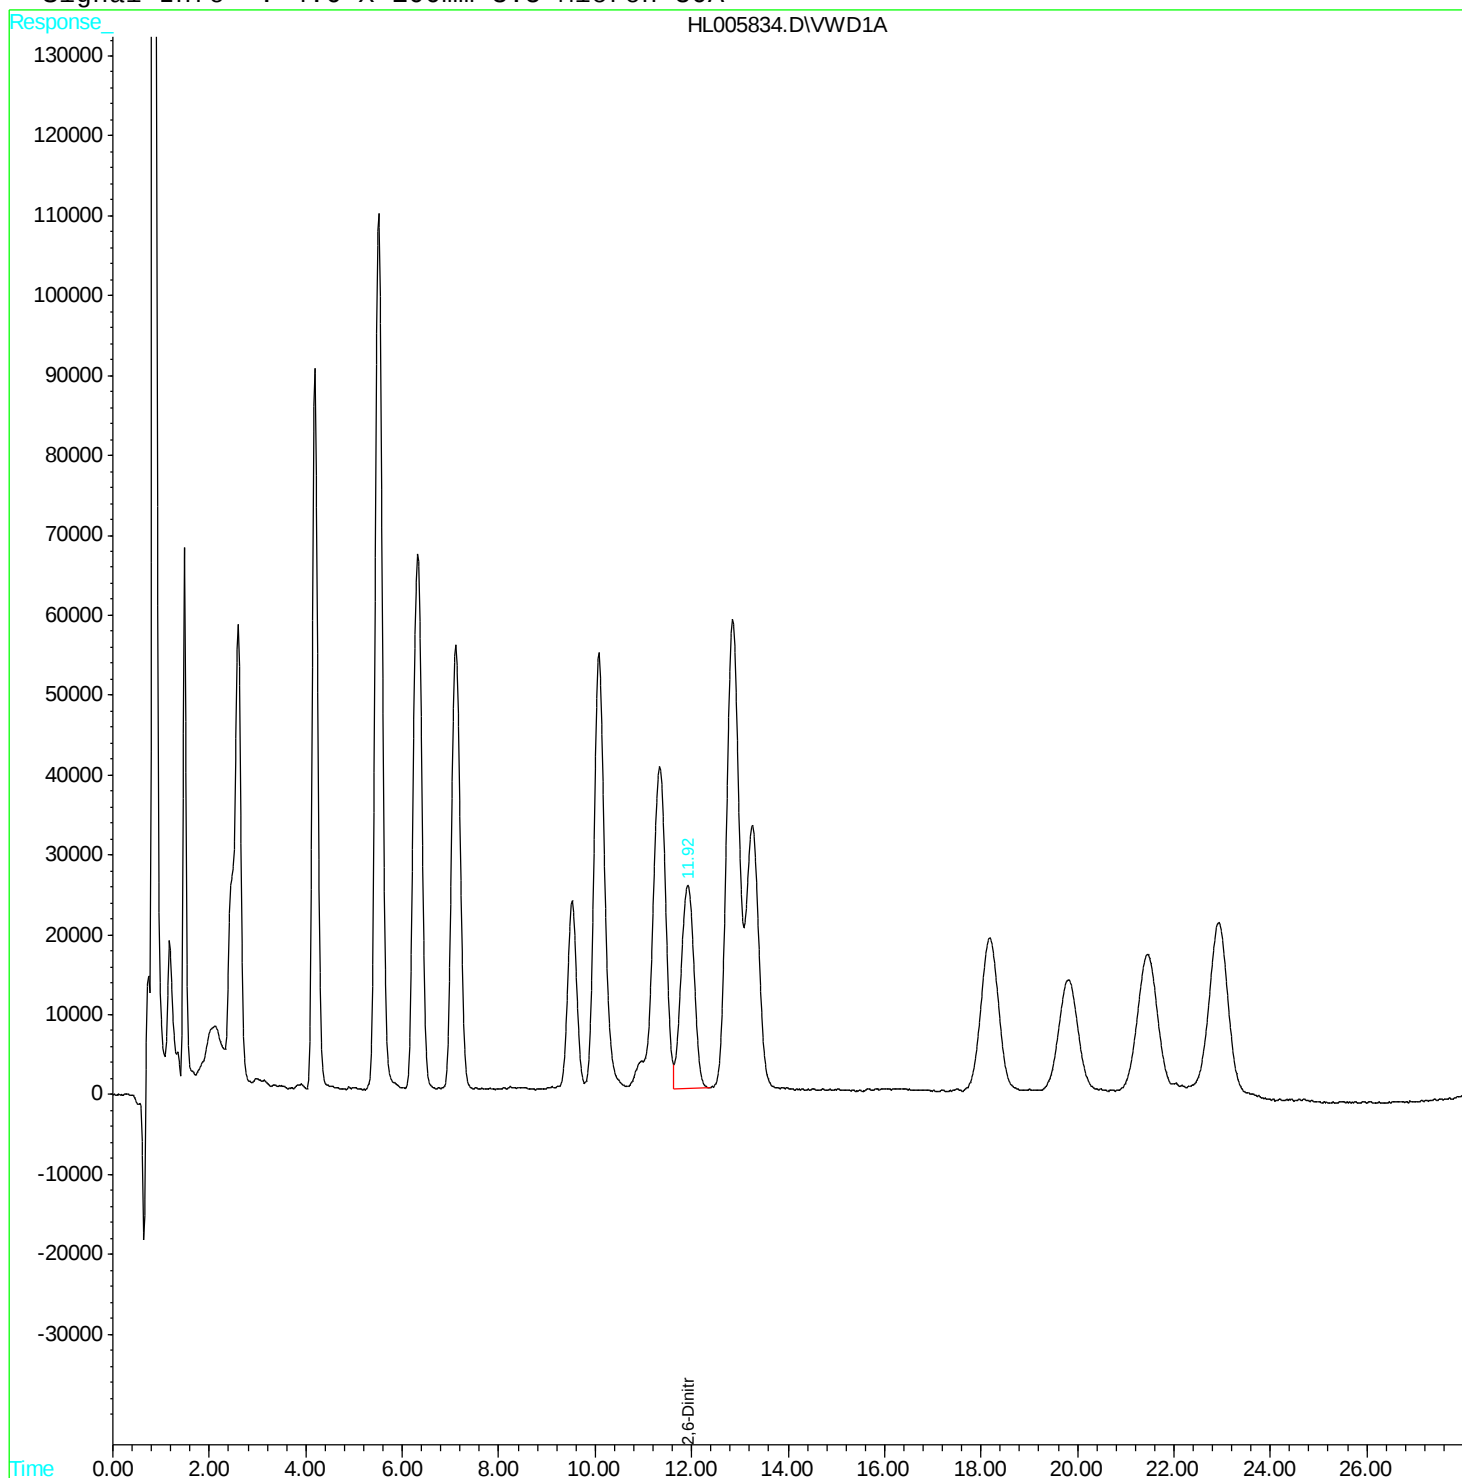


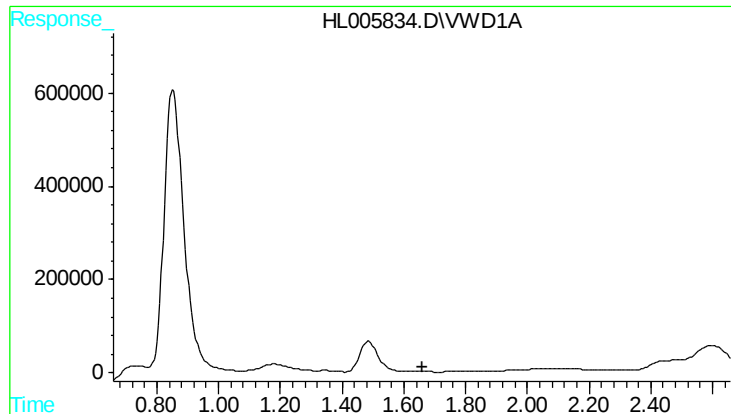

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 1.659 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

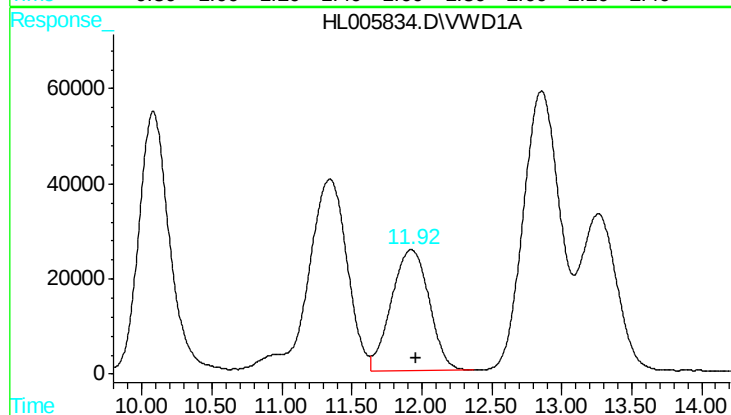

#13 2,6-Dinitrotoluene

R.T.: 11.924 min
Delta R.T.: -0.034 min
Response: 4776899
Conc: 410.22 ug/L