

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005845.D Vial: 1
Acq On : 05-Nov-2014, 01:55 Operator: TP
Sample : HSTDCCC0500 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 5 4:01 2014 Quant Results File: HL102214.RES

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Title :
Last Update : Fri Oct 25 15:16:02 2013
Response via : Initial Calibration
DataAcq Meth : TEST.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	2-Amino-4,6-dinitrotoluene	9.92	3110148	196.803 ug/L
-------	----------------------------	------	---------	--------------

Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.


HL005845.D HL102214.M Wed Nov 05 03:58:51 2014


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005845.D Vial: 1
Acq On : 05-Nov-2014, 01:55 Operator: TP
Sample : HSTDCCC0500 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 5 4:01 2014 Quant Results File: HL102214.RES

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Title :
Last Update : Fri Oct 25 15:16:02 2013
Response via : Multiple Level Calibration
DataAcq Meth : TEST.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

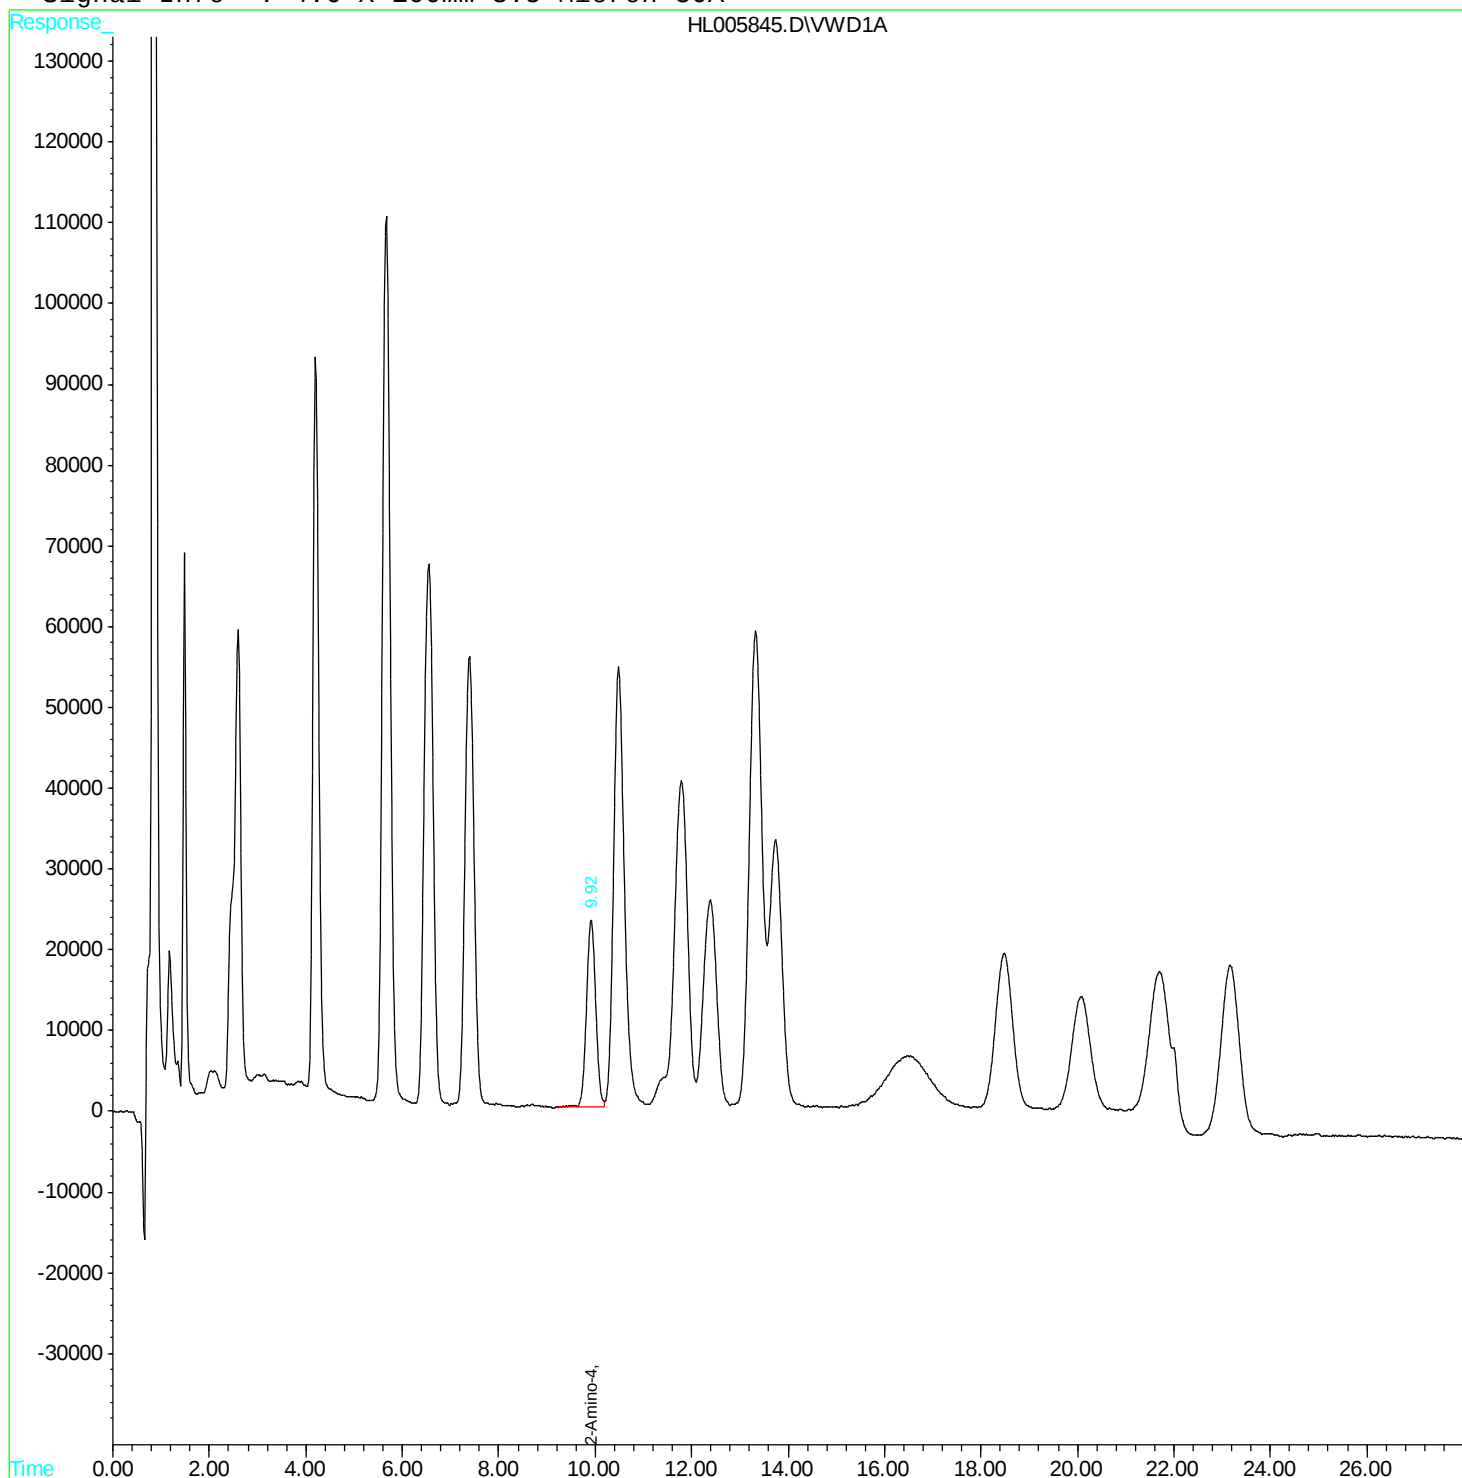


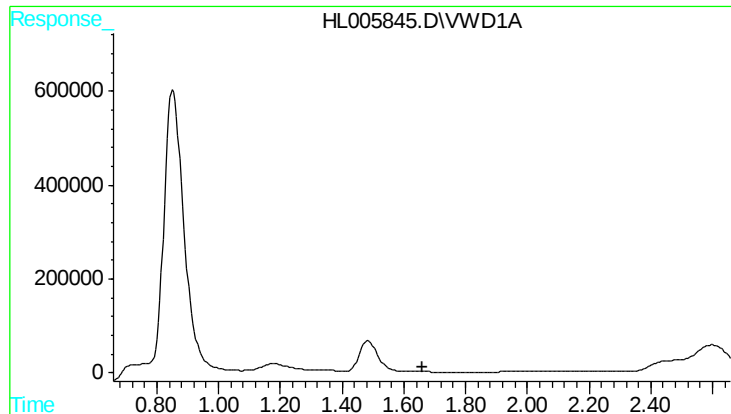

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 1.659 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

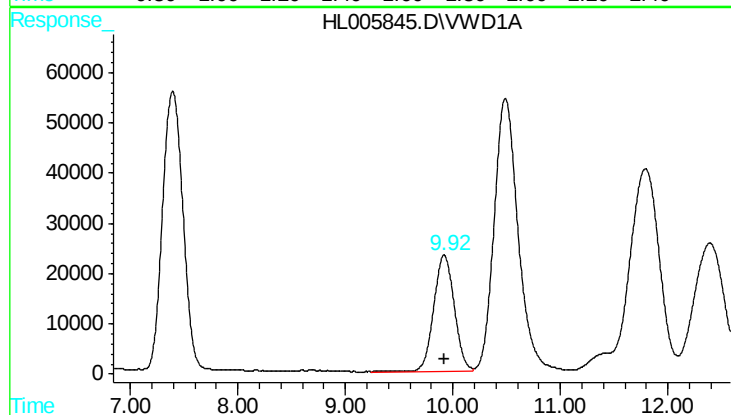

#10 2-Amino-4,6-dinitrotoluene

R.T.: 9.918 min
Delta R.T.: 0.002 min
Response: 3110148
Conc: 196.80 ug/L