

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005848.D Vial: 24
Acq On : 05-Nov-2014, 03:23 Operator: TP
Sample : F4351-06 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 5 6:48 2014 Quant Results File: HL102214.RES

Instrument :
HPLC_L
ClientSampleId :
YS19-SW04P-1014

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Title :
Last Update : Fri Oct 25 15:16:02 2013
Response via : Initial Calibration
DataAcq Meth : TEST.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) T RDX	2.10	235362	23.629 ug/L
6) T 3,5-Dinitroaniline	5.21	1439855	82.820 ug/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HL005848.D HL102214.M Wed Nov 05 06:46:02 2014


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005848.D Vial: 24
Acq On : 05-Nov-2014, 03:23 Operator: TP
Sample : F4351-06 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 5 6:48 2014 Quant Results File: HL102214.RES

Instrument :
HPLC_L
ClientSampleId :
YS19-SW04P-1014

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Title :
Last Update : Fri Oct 25 15:16:02 2013
Response via : Multiple Level Calibration
DataAcq Meth : TEST.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

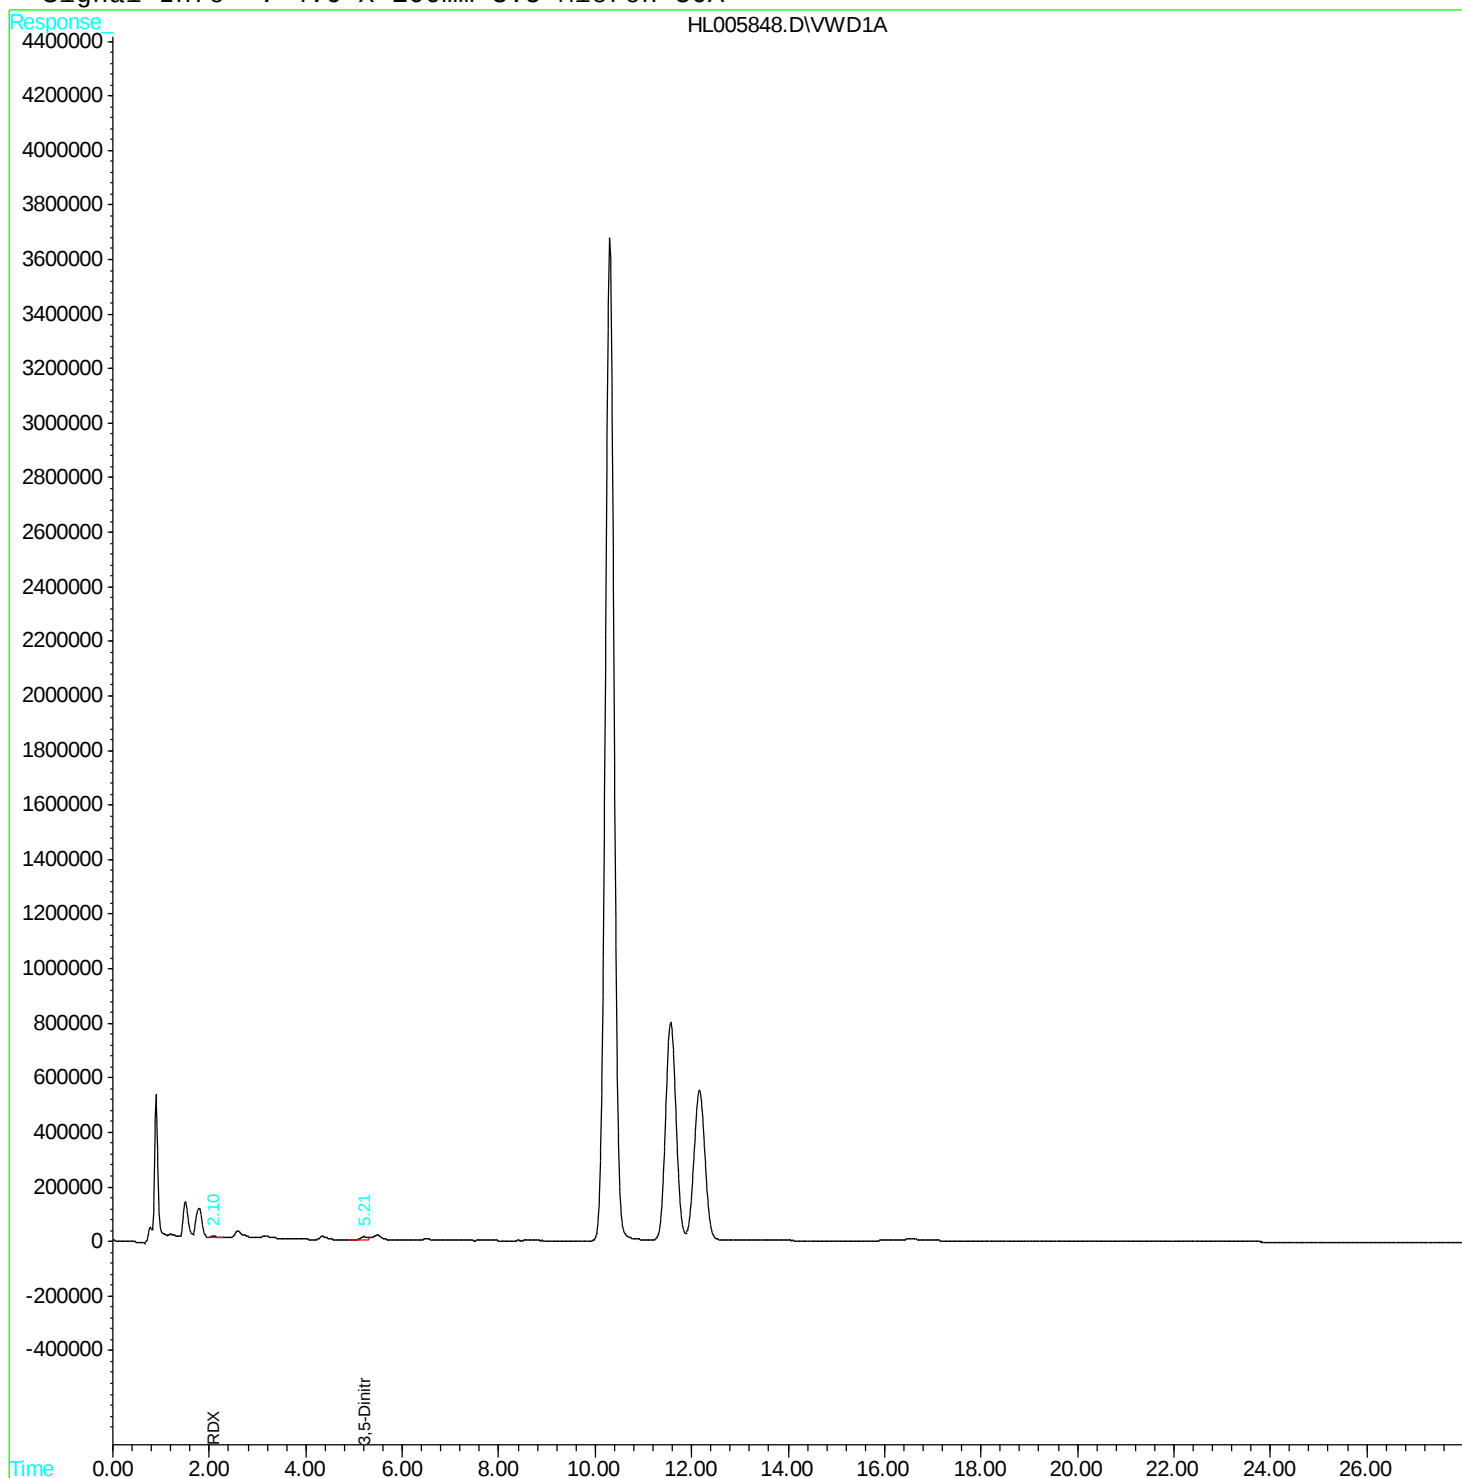


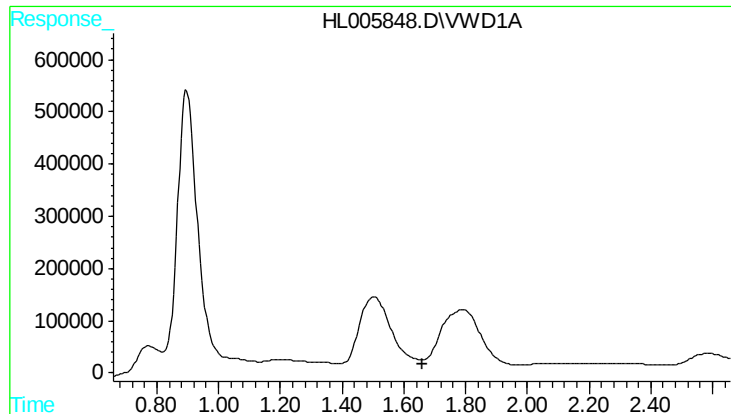

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 1.659 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
YS19-SW04P-1014

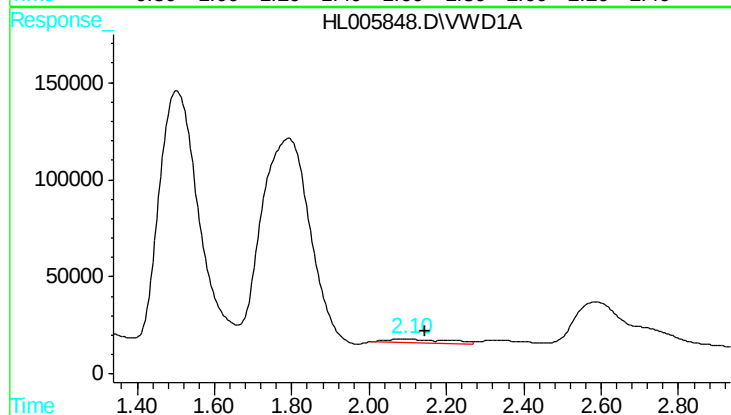

#3 RDX

R.T.: 2.095 min
Delta R.T.: -0.049 min
Response: 235362
Conc: 23.63 ug/L

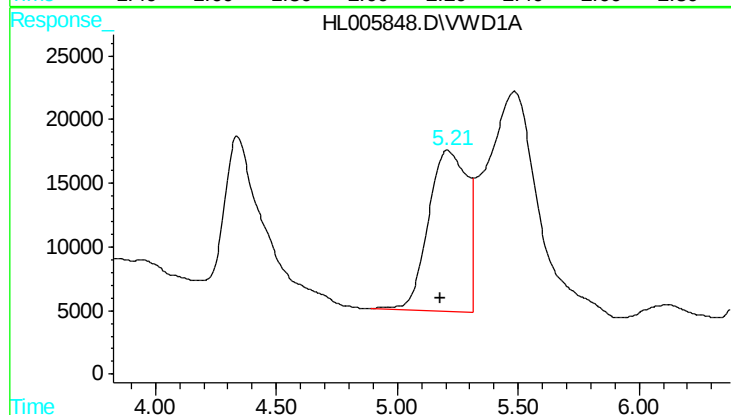

#6 3,5-Dinitroaniline

R.T.: 5.210 min
Delta R.T.: 0.031 min
Response: 1439855
Conc: 82.82 ug/L