

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005852.D Vial: 28
Acq On : 05-Nov-2014, 05:20 Operator: TP
Sample : F4351-12 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 5 6:48 2014 Quant Results File: HL102214.RES

Instrument :
HPLC_L
ClientSampleId :
YS19-EB01-101614-SW

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Title :
Last Update : Fri Oct 25 15:16:02 2013
Response via : Initial Calibration
DataAcq Meth : TEST.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

6) T	3,5-Dinitroaniline	5.13	598160	34.406 ug/L
------	--------------------	------	--------	-------------

Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.


HL005852.D HL102214.M Wed Nov 05 06:46:24 2014


Data File : Z:\HPCHEM1\HPLC_L\DATA\HL110414\HL005852.D Vial: 28
Acq On : 05-Nov-2014, 05:20 Operator: TP
Sample : F4351-12 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 5 6:48 2014 Quant Results File: HL102214.RES

Instrument :
HPLC_L
ClientSampleId :
YS19-EB01-101614-SW

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Title :
Last Update : Fri Oct 25 15:16:02 2013
Response via : Multiple Level Calibration
DataAcq Meth : TEST.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

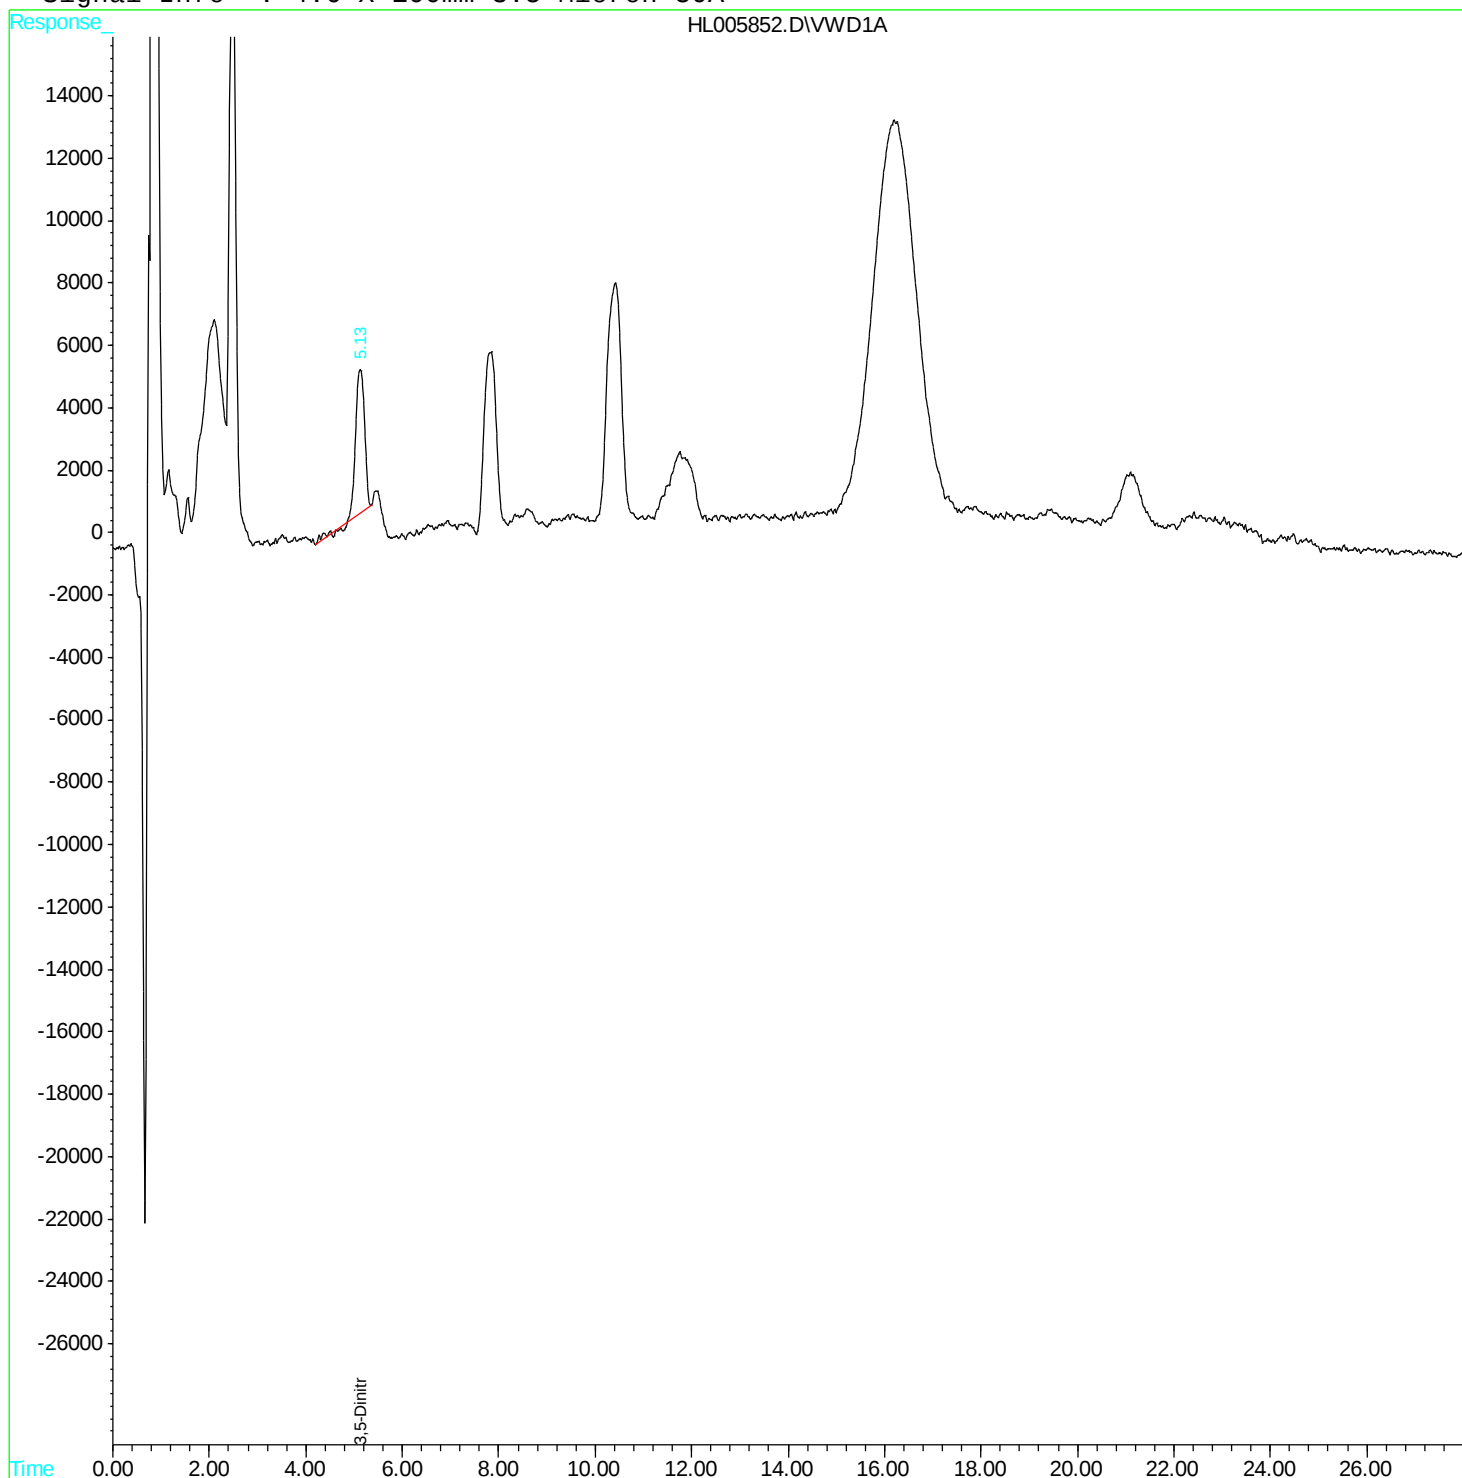


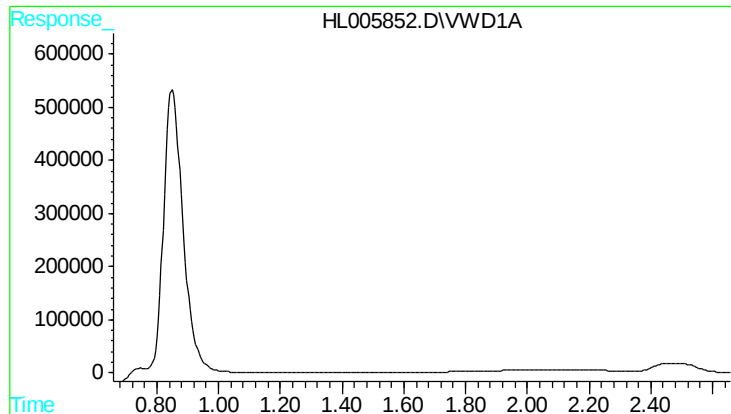

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 1.659 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :
YS19-EB01-101614-SW

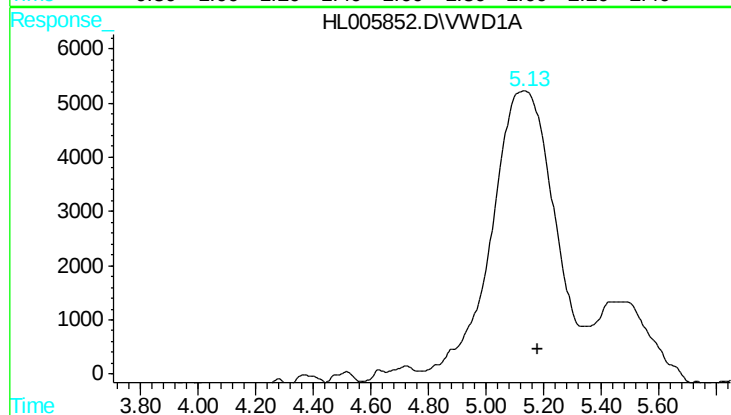

#6 3,5-Dinitroaniline

R.T.: 5.131 min
Delta R.T.: -0.048 min
Response: 598160
Conc: 34.41 ug/L