

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL110414\
 Data File : HL005862.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 05-Nov-2014, 09:44
 Operator : TP
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 HSTDCCC0500

Integration File signal 1: AUTOINT1.E
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 04:32:23 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
 Quant Title :
 QLast Update : Mon Mar 09 16:43:57 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	2.626	4764406	367.439 ug/L
Target Compounds			
2) T HMX	1.502	2779353	467.861 ug/L
3) T RDX	2.626	4764406	367.439 ug/L
4) T 1,3,5-Trinitrobenzene	4.230f	7118320	452.671 ug/L
11) T 4-Amino-2,6-dinitroto...	12.261f	5064102	494.607 ug/L
12) T 2,4-Dinitrotoluene	13.243	11131426	480.278 ug/L
13) T 2,6-Dinitrotoluene	13.671	6012842	512.994 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL110414\
Data File : HL005862.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 05-Nov-2014, 09:44
Operator : TP
Sample : HSTDCCC0500
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

Integration File signal 1: AUTOINT1.E
Integration File signal 2: autoint2.e
Quant Time: Mar 12 04:32:23 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Quant Title :
QLast Update : Mon Mar 09 16:43:57 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

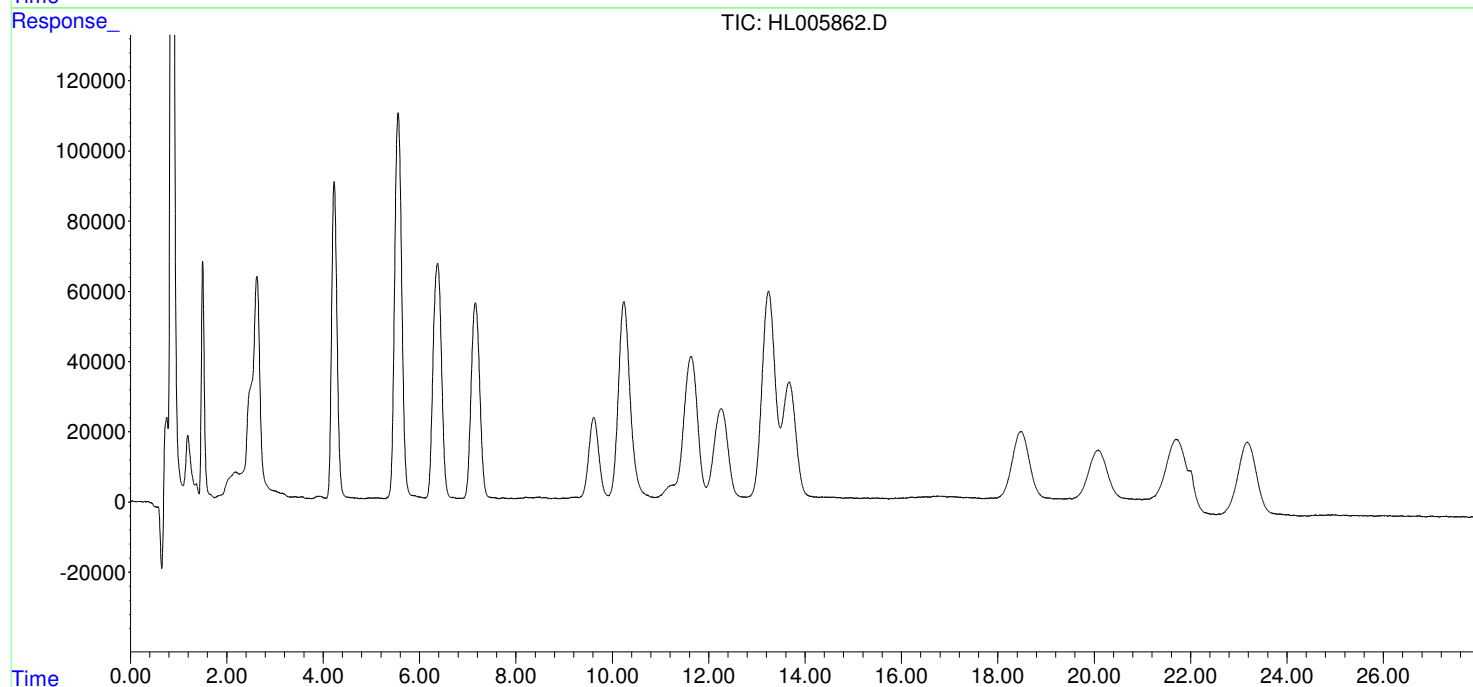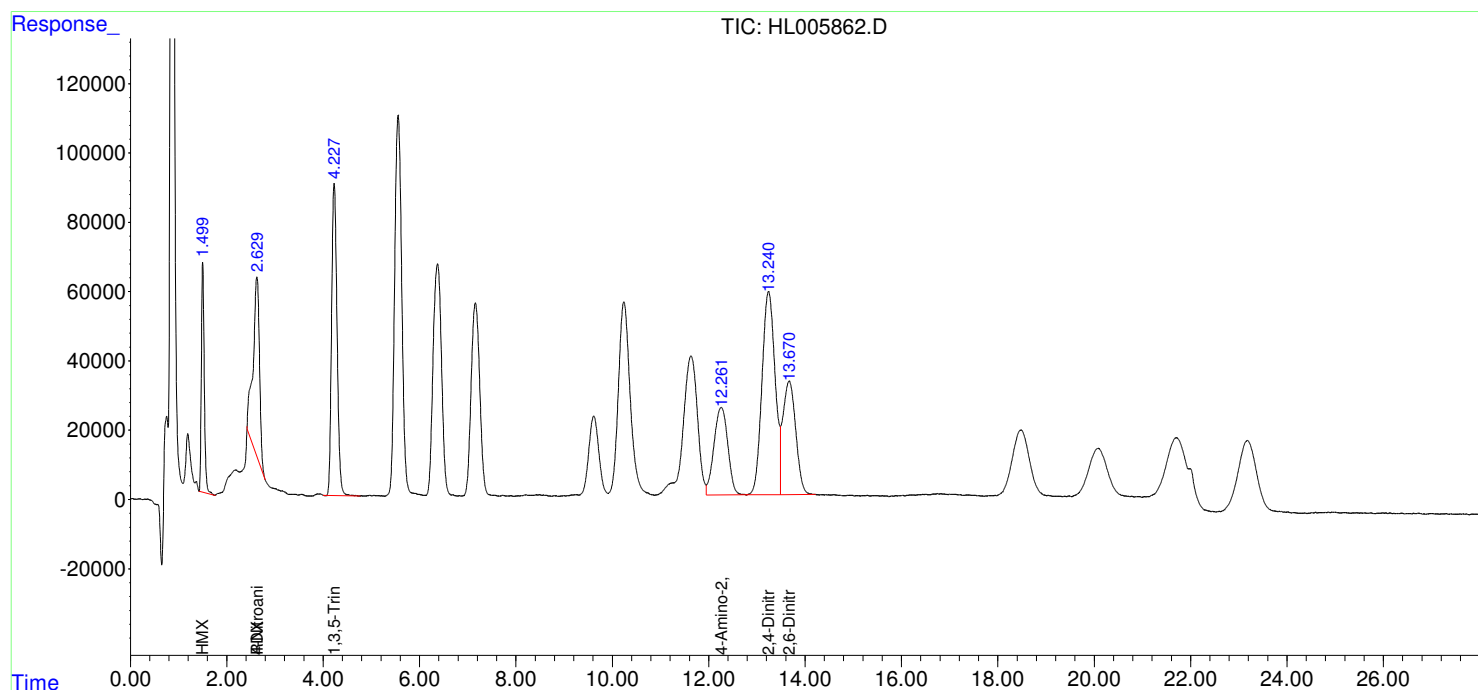


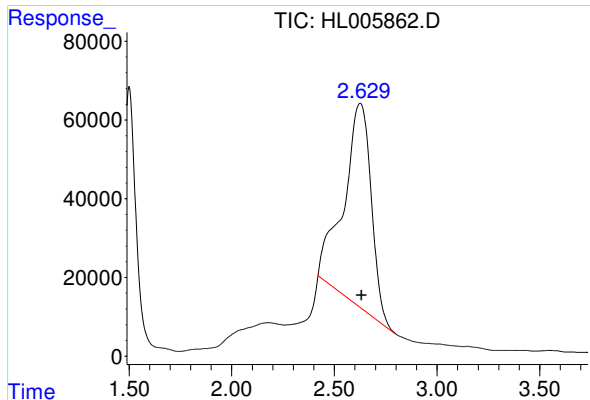

#1 4-Nitroaniline


R.T.: 2.626 min
Delta R.T.: -0.006 min
Response: 4764406
Conc: 367.44 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

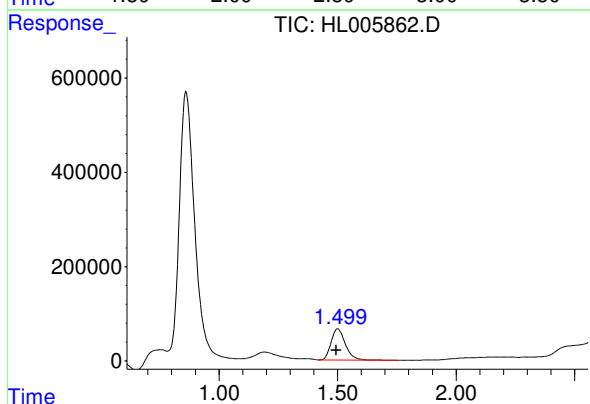


#2 HMX

R.T.: 1.502 min
Delta R.T.: 0.008 min
Response: 2779353
Conc: 467.86 ug/L

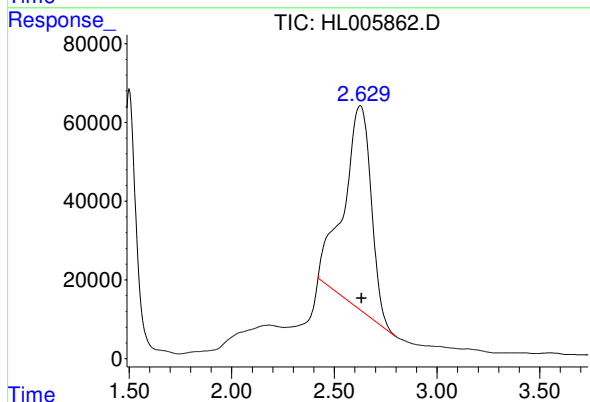


#3 RDX

R.T.: 2.626 min
Delta R.T.: -0.007 min
Response: 4764406
Conc: 367.44 ug/L

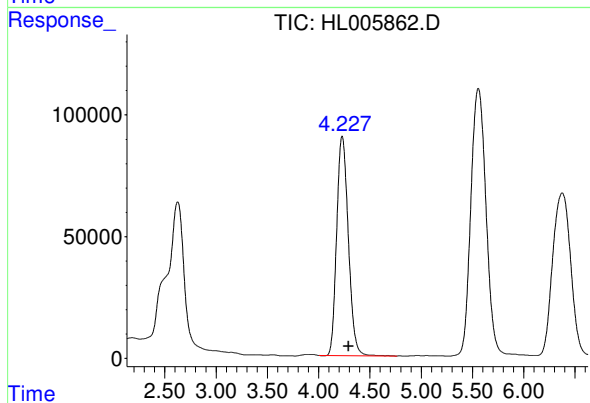

#4 1,3,5-Trinitrobenzene


R.T.: 4.230 min
Delta R.T.: -0.061 min
Response: 7118320
Conc: 452.67 ug/L

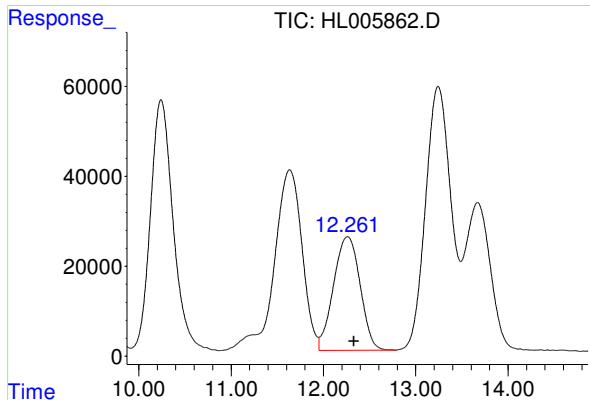

#11 4-Amino-2,6-dinitrotoluene


R.T.: 12.261 min
Delta R.T.: -0.068 min
Response: 5064102
Conc: 494.61 ug/L

Instrument :
HPLC_L
ClientSampleId :
HSTDCCC0500

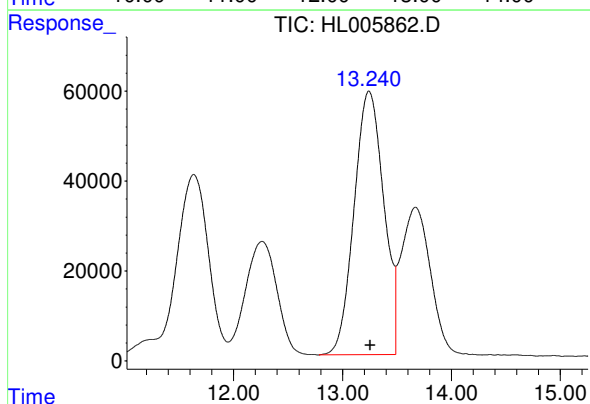

#12 2,4-Dinitrotoluene

R.T.: 13.243 min
Delta R.T.: -0.010 min
Response: 11131426
Conc: 480.28 ug/L

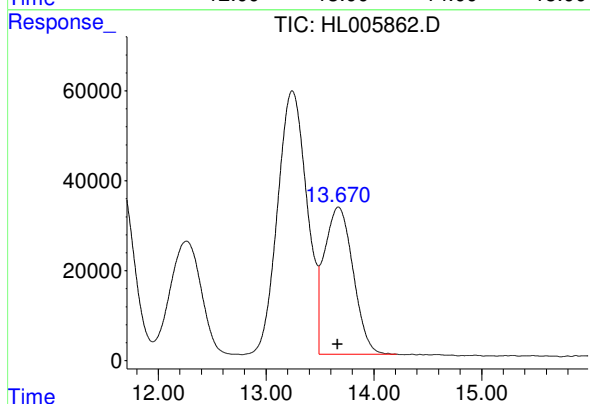

#13 2,6-Dinitrotoluene

R.T.: 13.671 min
Delta R.T.: 0.007 min
Response: 6012842
Conc: 512.99 ug/L