

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL110414\
 Data File : HL005826.D
 Signal(s) : VWD1A.CH
 Acq On : 04-Nov-2014, 16:37
 Operator : TP
 Sample : F4368-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 YS19-SB41-1014

Integration File: AUTOINT1.E
 Quant Time: Mar 09 17:08:56 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
 Quant Title :
 QLast Update : Mon Mar 09 17:08:54 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	2.503	1180200	91.019 ug/L
Target Compounds				
4) T	1,3,5-Trinitrobenzene	4.217	2351783	149.555 ug/L
9) T	2,4,6-Trinitrotoluene	10.128	838858849	57447.455 ug/L
10) T	2-Amino-4,6-dinitroto...	11.375	3920110	240.799 ug/L
11) T	4-Amino-2,6-dinitroto...	11.953	2542137	248.289 ug/L
12) T	2,4-Dinitrotoluene	12.888	381403	16.456 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL110414\
Data File : HL005826.D
Signal(s) : VWD1A.CH
Acq On : 04-Nov-2014, 16:37
Operator : TP
Sample : F4368-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
YS19-SB41-1014

Integration File: AUTOINT1.E
Quant Time: Mar 09 17:08:56 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Quant Title :
QLast Update : Mon Mar 09 17:08:54 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

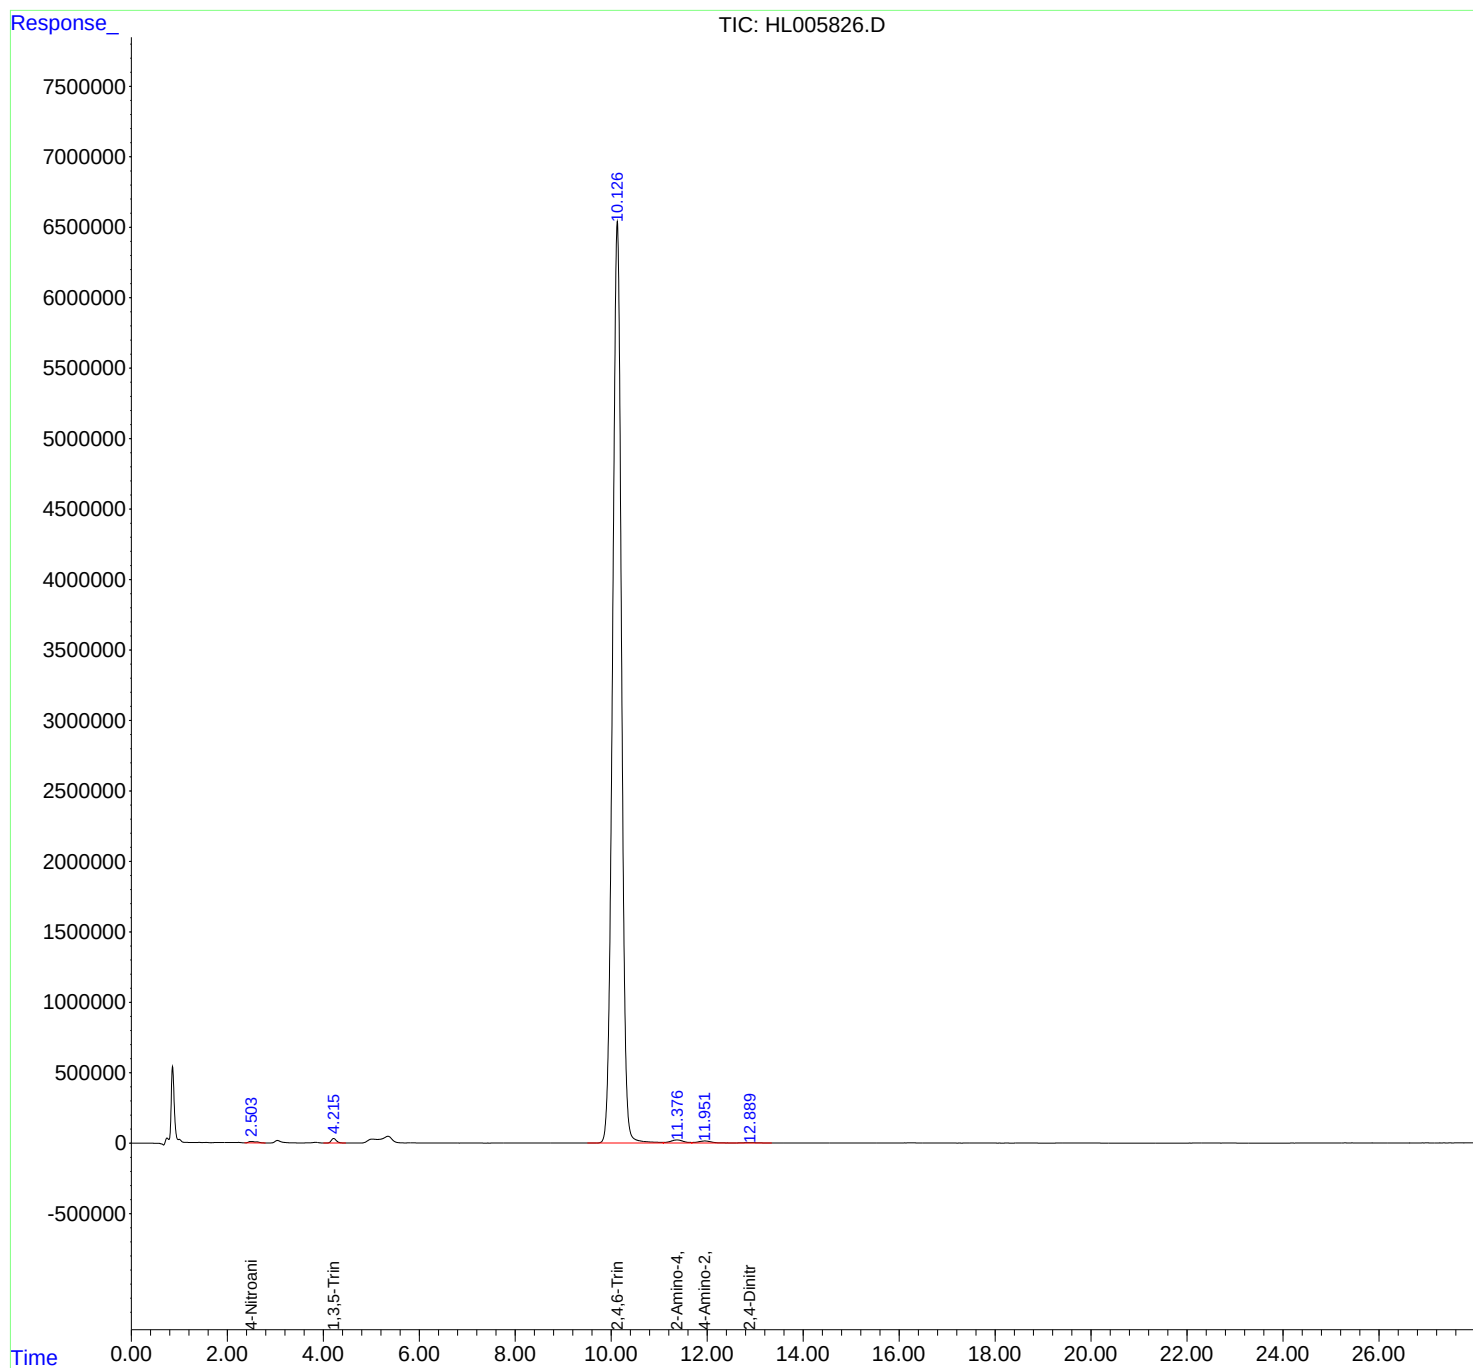


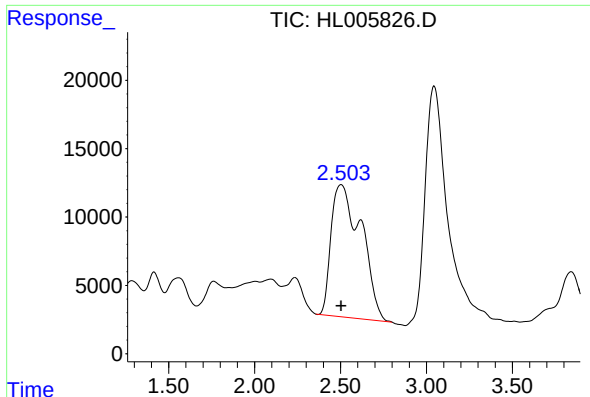

#1 4-Nitroaniline


R.T.: 2.503 min
Delta R.T.: 0.000 min
Response: 1180200
Conc: 91.02 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-SB41-1014

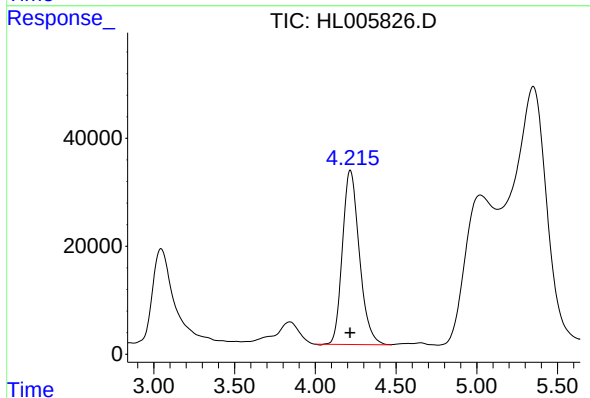


#4 1,3,5-Trinitrobenzene

R.T.: 4.217 min
Delta R.T.: 0.002 min
Response: 2351783
Conc: 149.56 ug/L

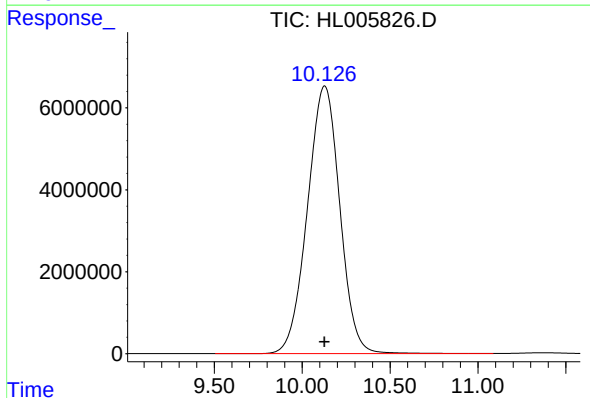


#9 2,4,6-Trinitrotoluene

R.T.: 10.128 min
Delta R.T.: 0.002 min
Response: 838858849
Conc: 57447.46 ug/L

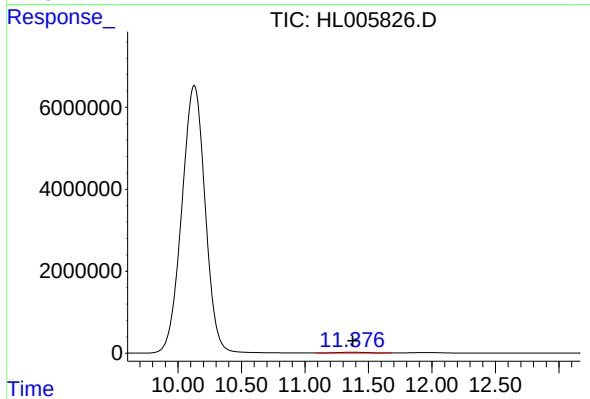

#10 2-Amino-4,6-dinitrotoluene


R.T.: 11.375 min
Delta R.T.: 0.000 min
Response: 3920110
Conc: 240.80 ug/L

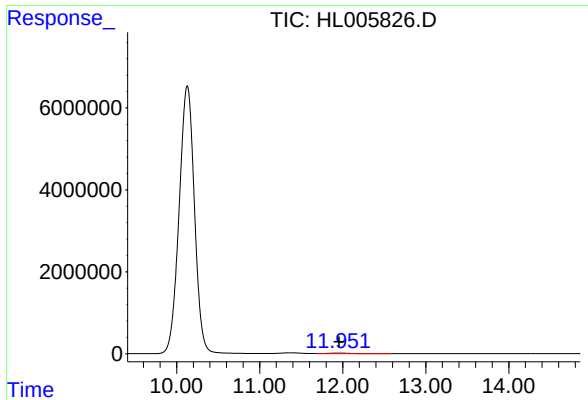

#11 4-Amino-2,6-dinitrotoluene

R.T.: 11.953 min
Delta R.T.: -0.002 min
Response: 2542137
Conc: 248.29 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-SB41-1014

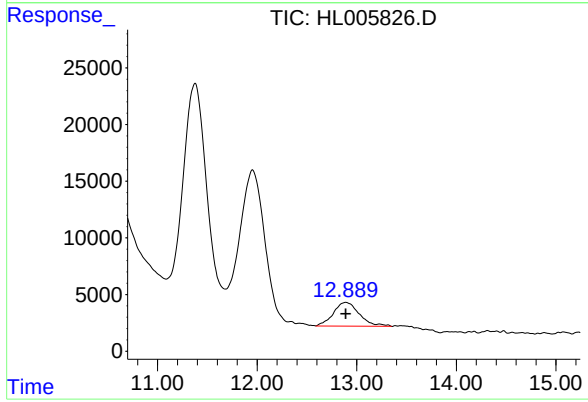

#12 2,4-Dinitrotoluene

R.T.: 12.888 min
Delta R.T.: 0.000 min
Response: 381403
Conc: 16.46 ug/L