

Data Path : Z:\HPCHEM1\HPLC_L\Data\HL110414\
 Data File : HL005836.D
 Signal(s) : VWD1A.CH
 Acq On : 04-Nov-2014, 21:31
 Operator : TP
 Sample : F4325-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 YS19-SS14-1014

Integration File: AUTOINT1.E
 Quant Time: Mar 09 14:18:22 2015
 Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
 Quant Title :
 QLast Update : Mon Mar 09 13:35:50 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	2.692	789481	60.886 ug/L
Target Compounds				
4) T	1,3,5-Trinitrobenzene	4.457	620320	39.448 ug/L
9) T	2,4,6-Trinitrotoluene	10.461	3925540	268.832 ug/L
10) T	2-Amino-4,6-dinitroto...	11.768	844785	51.892 ug/L
11) T	4-Amino-2,6-dinitroto...	12.290	738023	72.082 ug/L
12) T	2,4-Dinitrotoluene	13.268	441779	19.061 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_L\Data\HL110414\
Data File : HL005836.D
Signal(s) : VWD1A.CH
Acq On : 04-Nov-2014, 21:31
Operator : TP
Sample : F4325-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
YS19-SS14-1014

Integration File: AUTOINT1.E
Quant Time: Mar 09 14:18:22 2015
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL102214.M
Quant Title :
QLast Update : Mon Mar 09 13:35:50 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

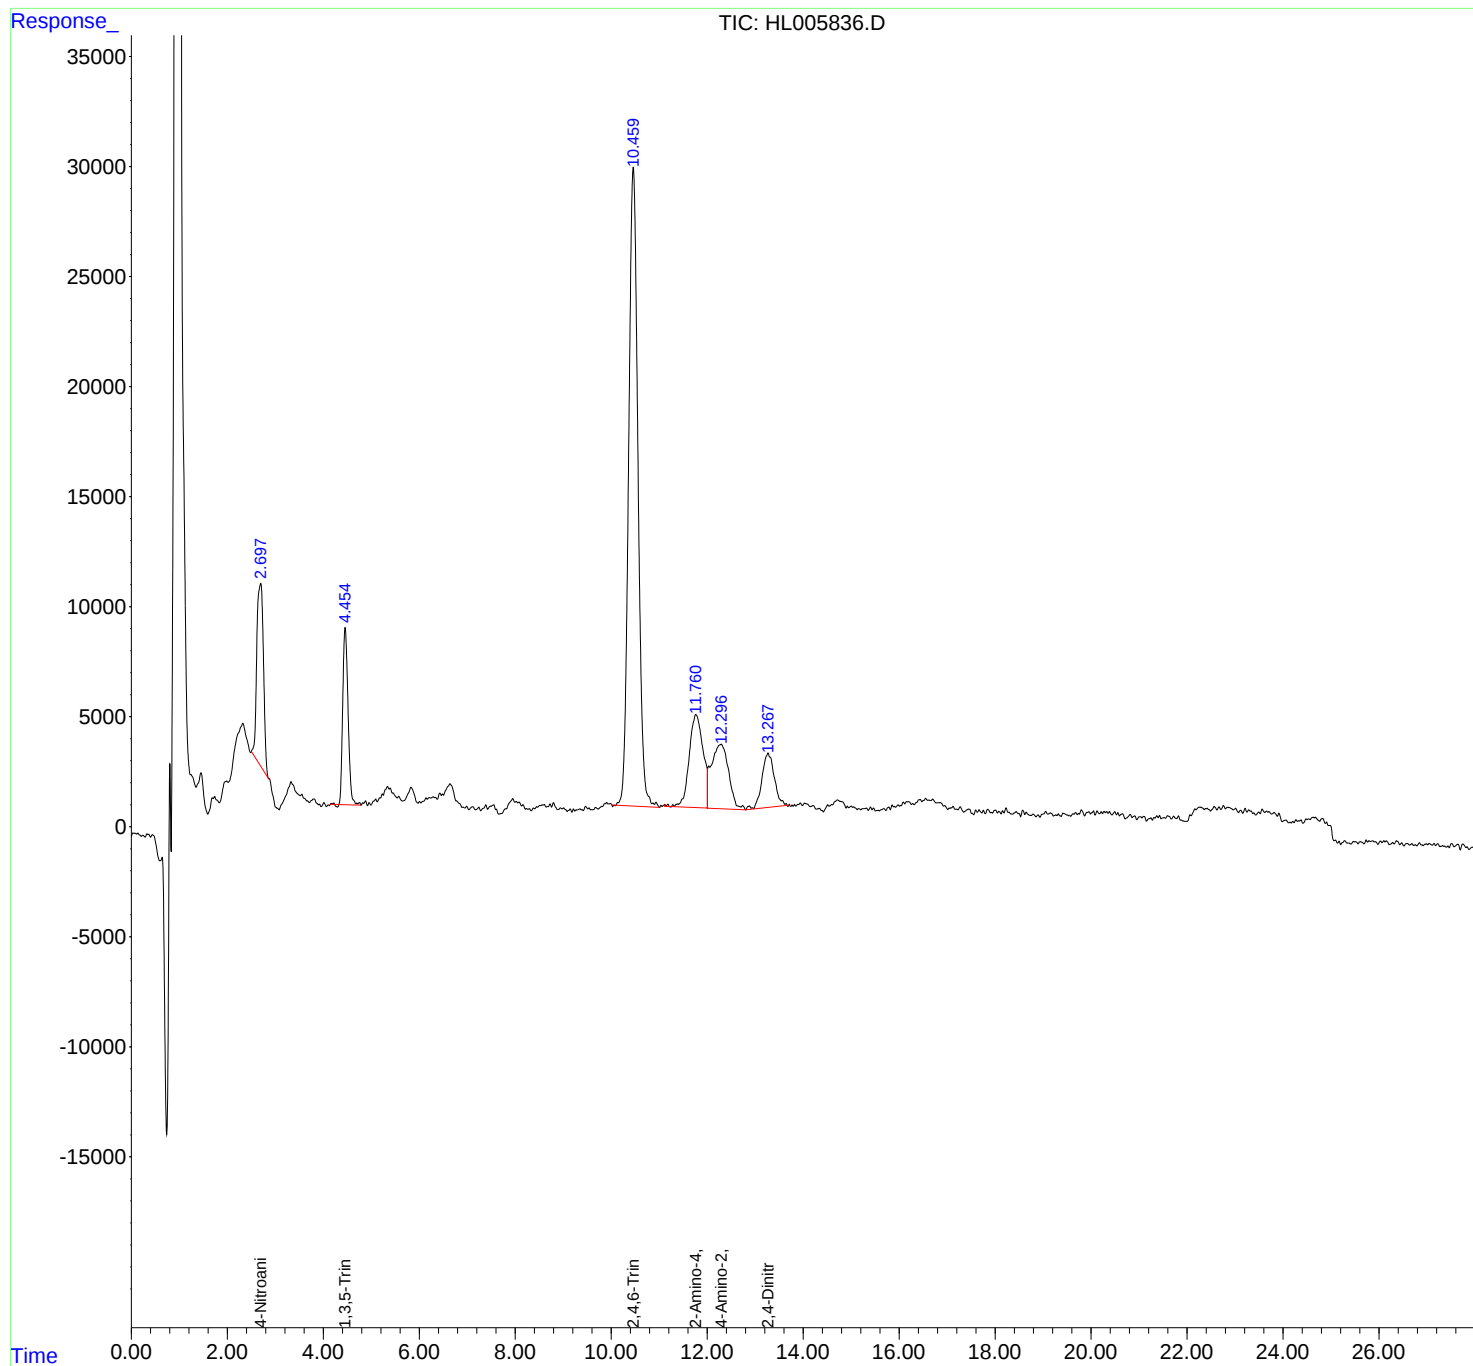


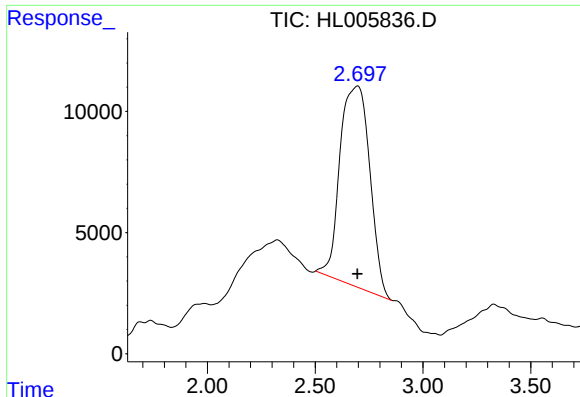

#1 4-Nitroaniline


R.T.: 2.692 min
Delta R.T.: -0.005 min
Response: 789481
Conc: 60.89 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-SS14-1014

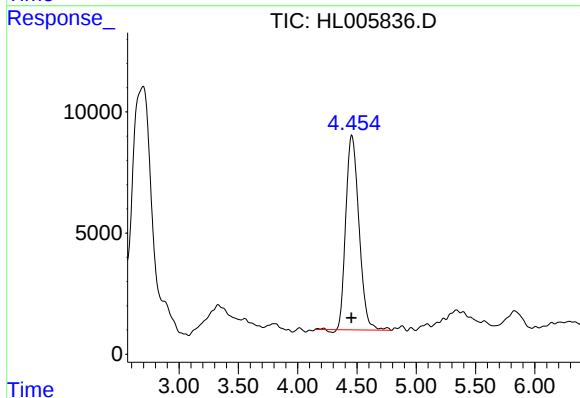


#4 1,3,5-Trinitrobenzene

R.T.: 4.457 min
Delta R.T.: 0.003 min
Response: 620320
Conc: 39.45 ug/L

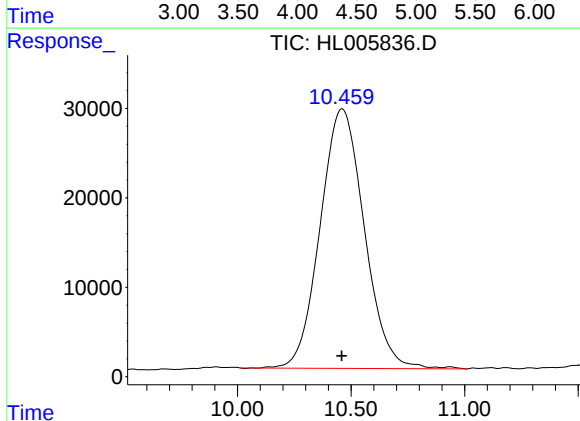


#9 2,4,6-Trinitrotoluene

R.T.: 10.461 min
Delta R.T.: 0.002 min
Response: 3925540
Conc: 268.83 ug/L

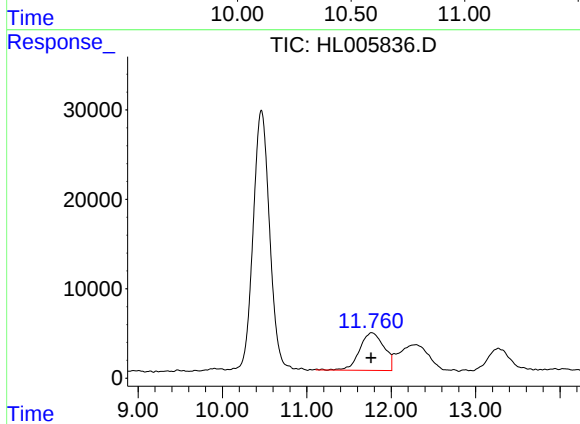

#10 2-Amino-4,6-dinitrotoluene


R.T.: 11.768 min
Delta R.T.: 0.008 min
Response: 844785
Conc: 51.89 ug/L

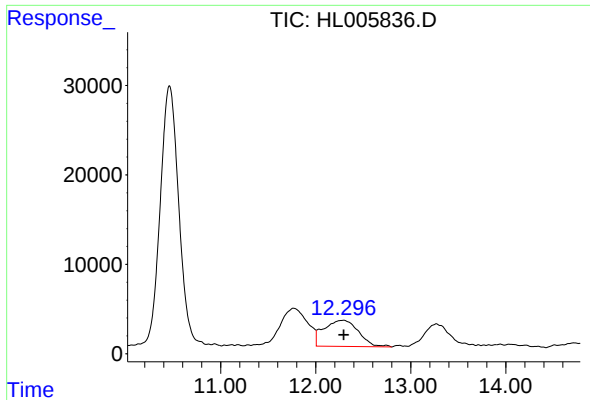

#11 4-Amino-2,6-dinitrotoluene

R.T.: 12.290 min
Delta R.T.: -0.006 min
Response: 738023
Conc: 72.08 ug/L

Instrument :
HPLC_L
ClientSampleId :
YS19-SS14-1014

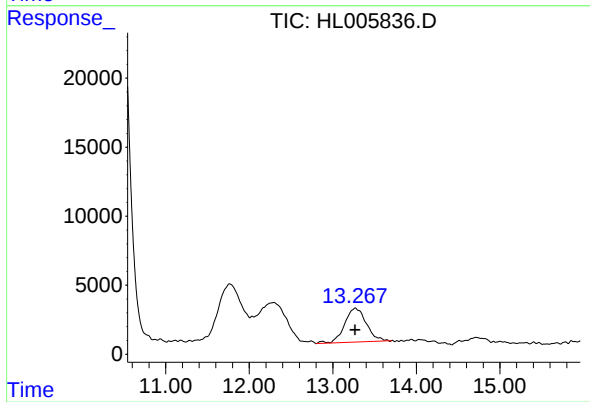

#12 2,4-Dinitrotoluene

R.T.: 13.268 min
Delta R.T.: 0.000 min
Response: 441779
Conc: 19.06 ug/L